



Workshop in Diagnostic Immunohistochemistry
Aalborg University Hospital, September 19th – 21st 2016

Immunohistochemical principles

The technical test approach


Post-analytical phase

Controls


Søren Nielsen
Project coordinator & Scheme Manager
NordiQC
Aalborg University Hospital, Denmark

IHC – Biomarker controls

... The biomarker protocol trap – Caution: not for faint-hearted lab personel !!!!!

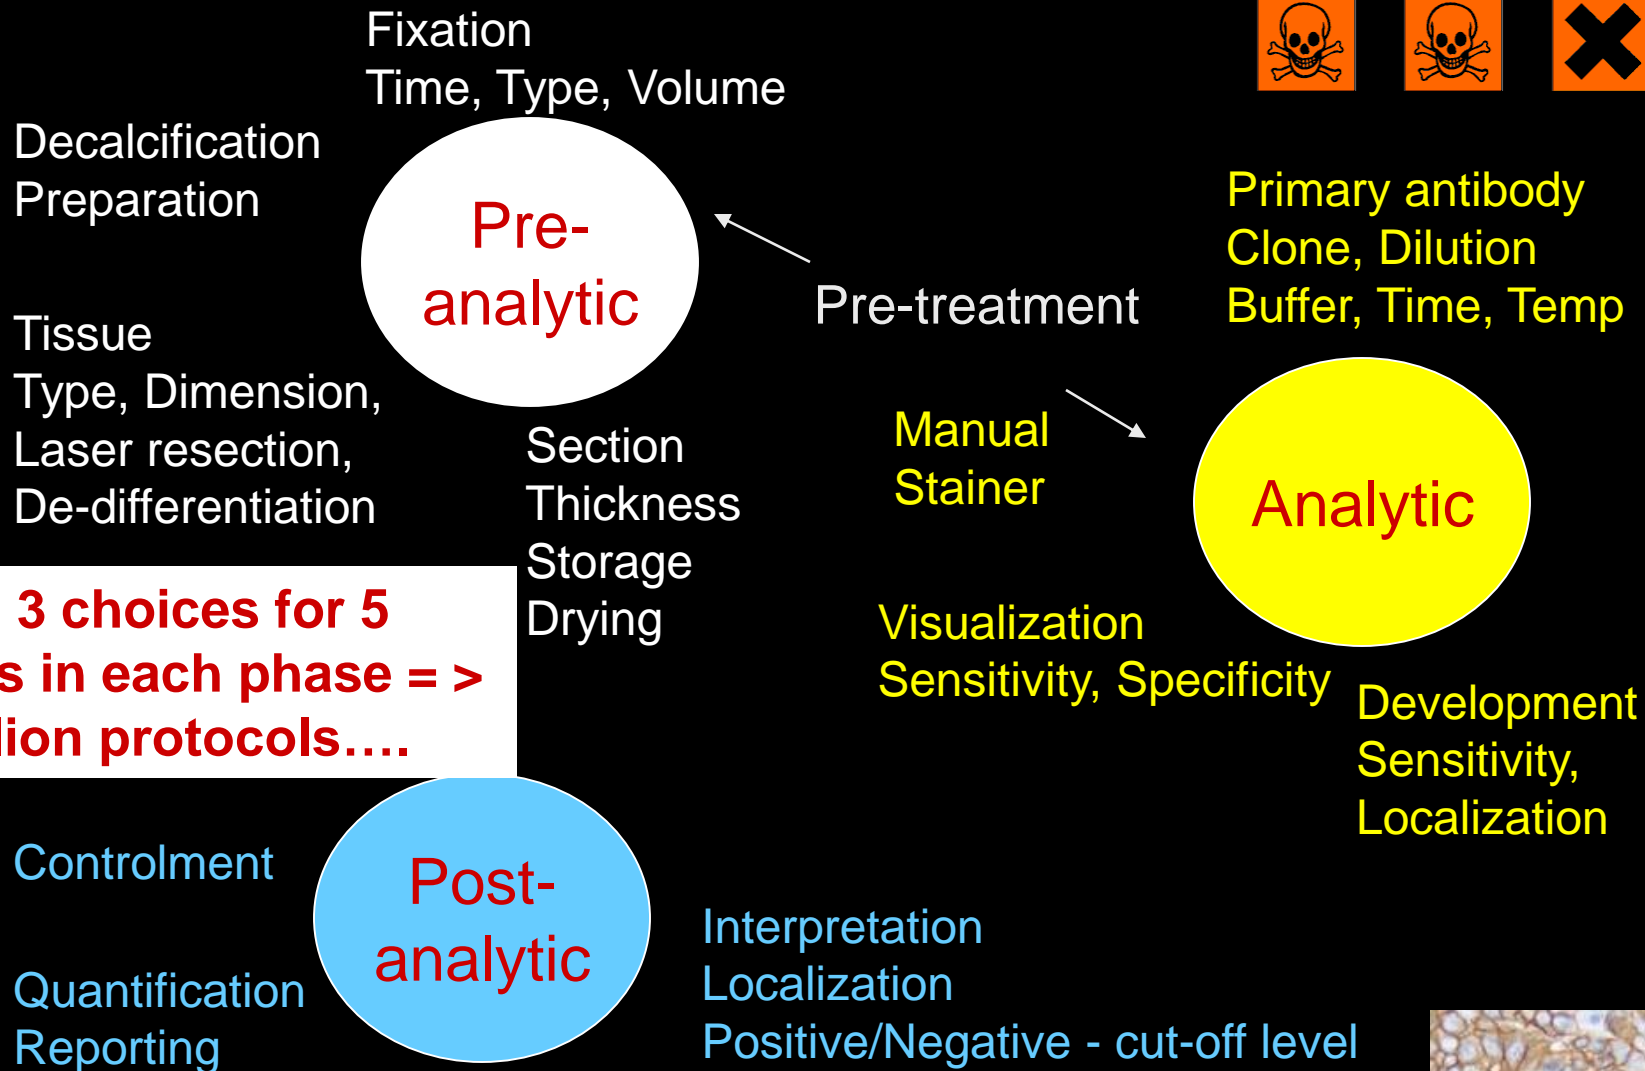

The right control material will expose right or wrong choices



- What is an IHC control in diagnostic IHC ?
- What is recommended and best practice ?
- What are the pitfalls for the use of IHC controls ?
- How can IHC controls be used by laboratories & EQA ?
- How to use IHC controls to implement new markers.

REVIEW ARTICLE

Appl Immunohistochem Mol Morphol . Volume 22, Number 4, October 2014

Standardization of Negative Controls in Diagnostic Immunohistochemistry: Recommendations From the International Ad Hoc Expert Panel

Emina E. Torlakovic, MD, PhD,†‡ Glenn Francis, MBBS, FRCPA, MBA, FFSc (RCPA),§¶
John Garratt, RT,†‡## Blake Gilks, MD, FRCPC,†‡** Elizabeth Hyjek, MD, PhD,*
Merdol Ibrahim, PhD,†† Rodney Miller, MD,‡‡ Soren Nielsen, HT, CT,§§||
Eugen B. Petcu, MD, PhD,§ Paul E. Swanson, MD,¶¶ Clive R. Taylor, MD, PhD,##
and Mogens Vyberg, MD§§||*

REVIEW ARTICLE

Appl Immunohistochem Mol Morphol • Volume 23, Number 1, January 2015

Standardization of Positive Controls in Diagnostic Immunohistochemistry: Recommendations From the International Ad Hoc Expert Committee

Emina E. Torlakovic, MD, PhD,† Soren Nielsen, HT, CT,‡§ Glenn Francis, MBBS, FRCPA,
MBA, FFSc (RCPA),||¶## John Garratt, RT,†** Blake Gilks, MD, FRCPC,†††
Jeffrey D. Goldsmith, MD,‡‡ Jason L. Hornick, MD, PhD,*§§ Elizabeth Hyjek, MD, PhD,*
Merdol Ibrahim, PhD,|| Keith Miller, FIBMS,|| Eugen Petcu, MD, PhD,||
Paul E. Swanson, MD,¶¶## Xiaoge Zhou, MD,***††† Clive R. Taylor, MD, PhD,‡‡‡
and Mogens Vyberg, MD‡§*

Abstract: Diagnostic immunohistochemistry (dIHC) has been practiced for several decades, with an ongoing expansion of applications for diagnostic use, and more recently for detection of prognostic and predictive biomarkers. However, standardization of practice has not to be achieved, despite significant

mittee has clarified definitions of IHC assay sensitivity and specificity, with special emphasis on how these definitions apply to positive controls. Recommendations for “best laboratory practice” regarding positive controls for dIHC are specified. The first set of immunohistochemistry critical assay performance


Documentation of Immunocytochemistry Controls in the Cytopathologic Literature: A Meta-Analysis of 100 Journal Articles

Diagnostic Cytopathology, Vol 39, No 4

2011

Carol Colasacco, M.L.I.S., S.C.T.(A.S.C.P.), C.T.(I.A.C.),^{1*} Sharon Mount, M.D.,^{1,2}
and Gladwyn Leiman, M.B.B.C.H., F.I.A.C., F.R.C.Path.^{1,2}

ICC Controls in the Literature

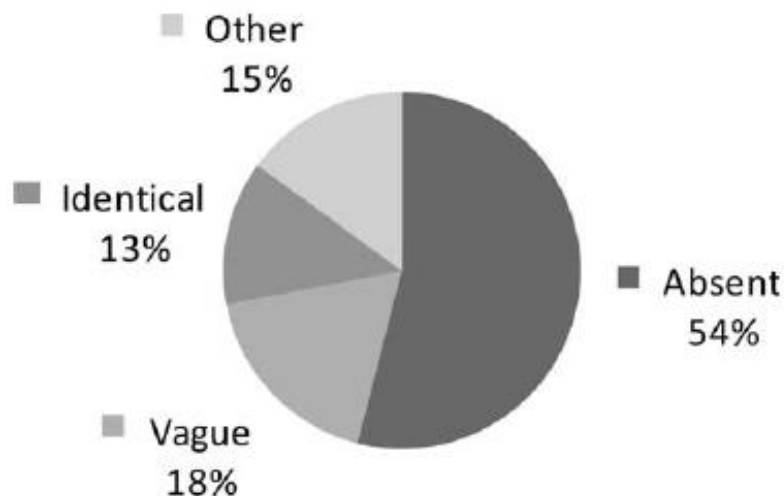

Absent: Controls were not mentioned.

Vague: Statement such as “appropriate positive and negative controls were included.”

Identical: Controls identical to study samples were described.

Other: Controls were dissimilar or partially similar (i.e., tissue control with smears or tissue control with cell block and ThinPrep samples run), or samples were too scant to include controls.

> 70 % of publications based on IHC do not describe controls used to verify data and conclusions....

Fig. 1. Description of immunocytochemistry controls in articles reviewed.

J Neurooncol (2014) 119:39–47
DOI 10.1007/s11060-014-1459-5

1' publication with this finding

LABORATORY INVESTIGATION

Till 2014; EpCAM not seen in glioma

The overexpression of Epithelial cell adhesion molecule (EpCAM) in glioma

Xin Chen · Wei-Yuan Ma · Shang-Chen Xu · Yu Liang · Yi-Bing Fu ·
Bo Pang · Tao Xin · Hai-Tao Fan · Rui Zhang · Jian-Gang Luo ·
Wen-Qing Kang · Min Wang · Qi Pang

“Immunohistochemistry results showed EpCAM was widely expressed in glioma (90.8 %).

The overall survival of WHO III and IV glioma patients with EpCAM overexpression was obviously lower than that without EpCAM overexpression. EpCAM overexpression was an independent prognostic factor for overall survival in glioma patients.

This study firstly shows that EpCAM overexpression correlates significantly with malignancy (WHO grades), proliferation (Ki67), angiogenesis (MVD), and prognosis in gliomas.”

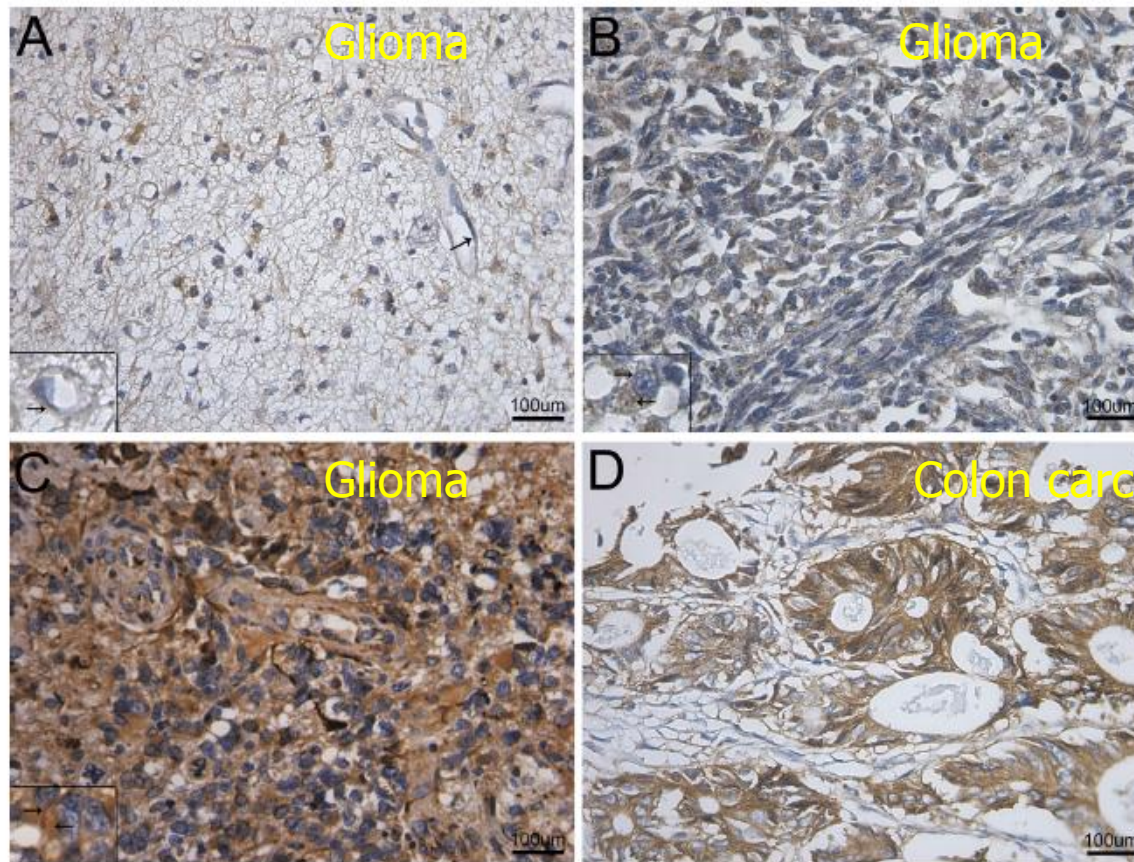


Fig. 1 Representative immunohistochemical staining for EpCAM (400×). Membranous and Cytoplasmic staining of EpCAM was observed in (a-c); a WHO grade II malignant glioma with weak EpCAM expression(TIS = 4), slant arrow shows EpCAM staining on epithelial cell; b WHO grade III malignant glioma with moderate EpCAM expression(TIS = 8); c WHO grade IV with intense EpCAM

expression(TIS = 12). d intense membranous staining in intestine adenocarcinoma was showed as a positive control. Inserts show representative staining; Left-to-right arrows show membranous staining and right-to-left arrows show cytoplasmic staining.WHO, World Health Organization, *EpCAM* epithelial cell adhesion molecule, *TIS* total immunostaining score

Method – sensitivity, specificity – antibody, retrieval etc ?
Material – handling, processing, selected etc?
Interpretation – cut-off values, localization etc ?

Methods:

Polyclonal antibody towards EpCAM – Abcam ab 71916

- HIER Citrate pH 6 for 20 min. At 98°C
- 1:100, 16 hours incubation at 4°C
- 3-step polymer based detection system

Positive (tissue) control: Colon adenocarcinoma

Negative (reagent) control: Omission of primary antibody


Cut-off was 1% positivity – any intensity; "overexpression $\geq 10\%$ and mod.

"Immunohistochemistry results showed EpCAM was widely expressed in glioma (90.8 %)."



IHC – Biomarker controls

Ref. NordiQC: Ber-EP4: 1:50, HIER TRS pH 6.1, 3-step polymer


Glioma

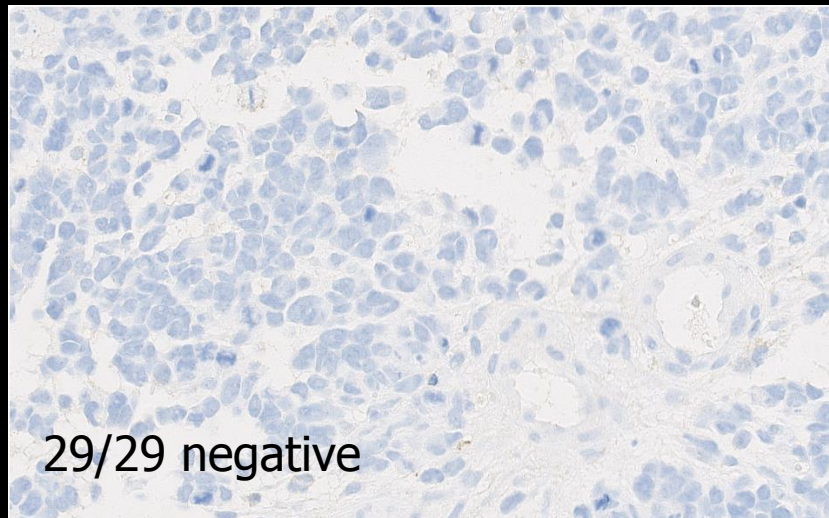

Kidney

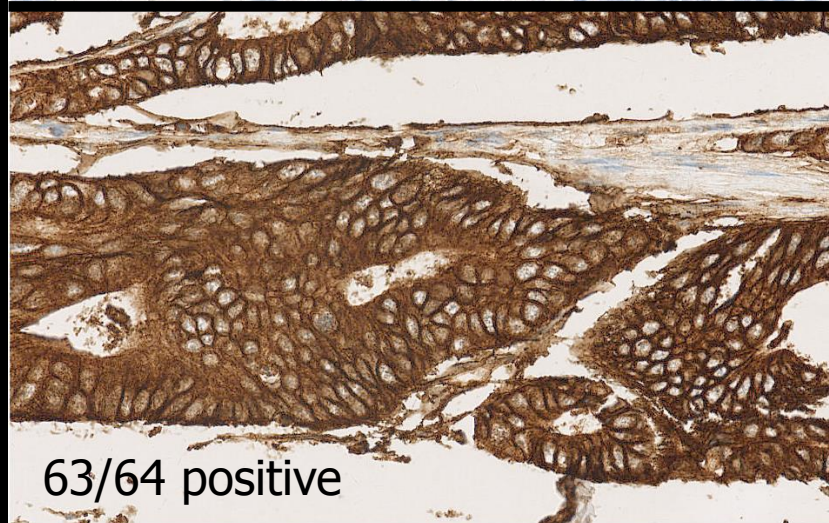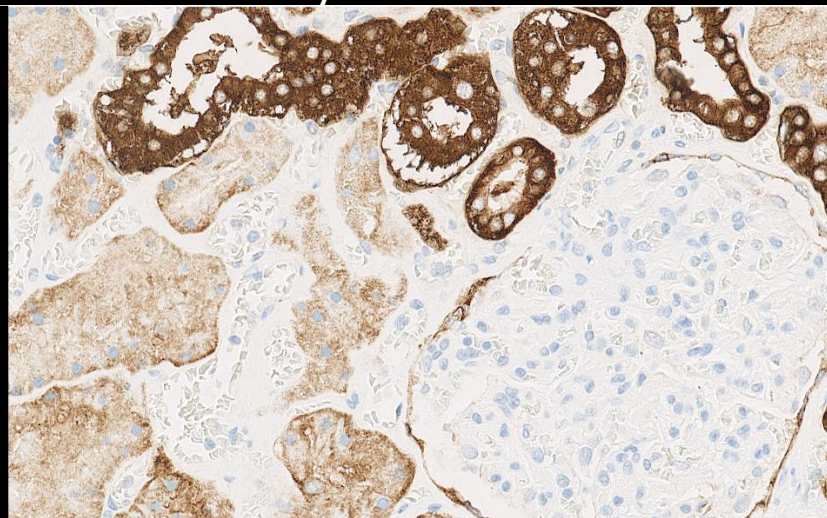

Colon ad. carc.

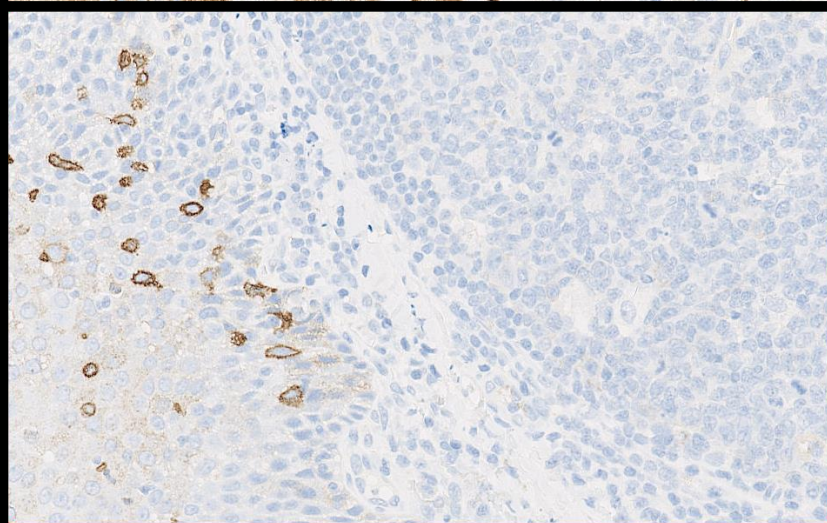


Tonsil



IHC – Biomarker controls

Study: Abcam ab 71916: 1:100, HIER TRS pH 6.1, 3-step polymer


Glioma

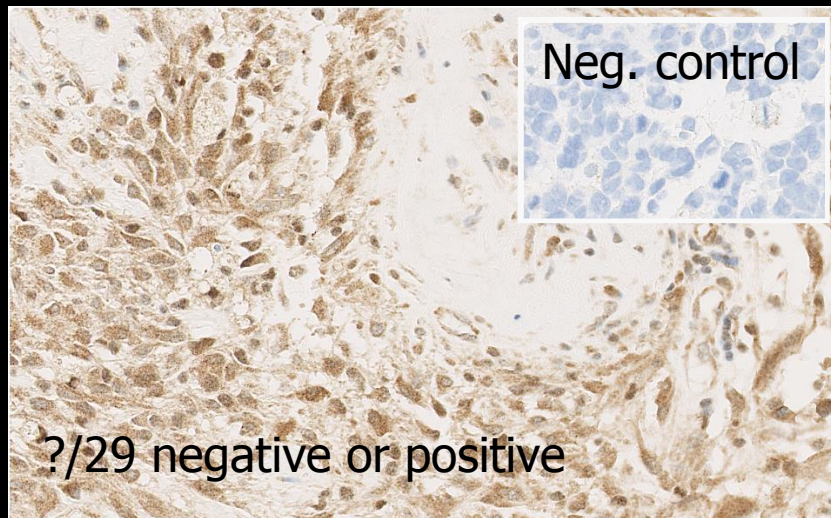

Kidney

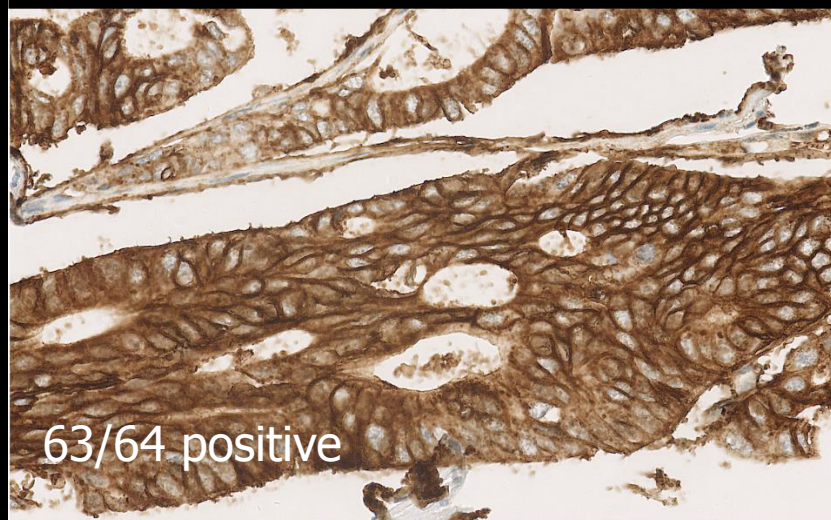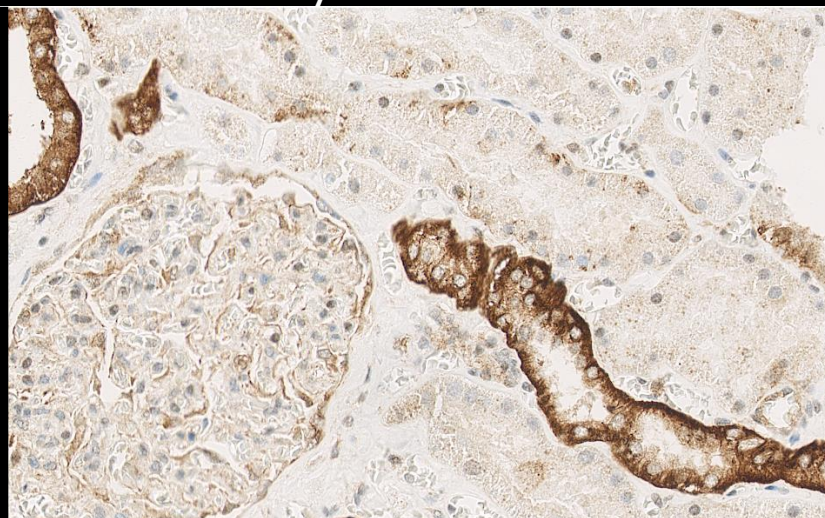


Colon ad. carc.

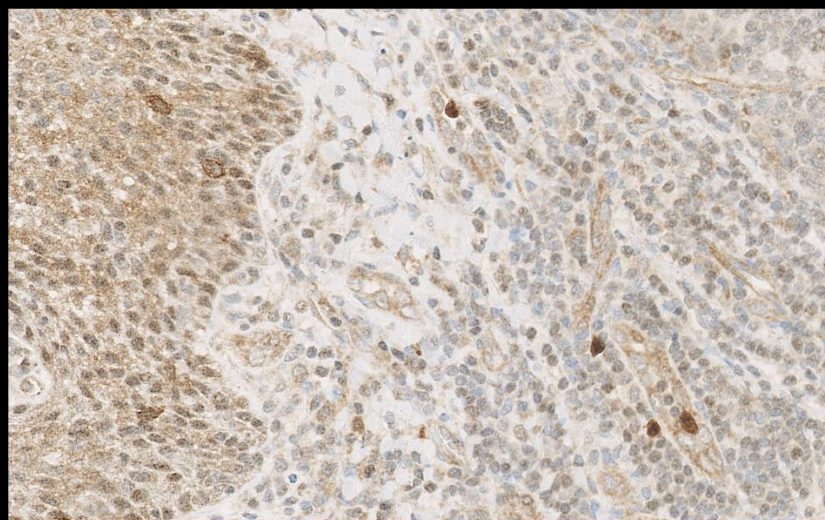


Tonsil

IHC – Biomarker controls

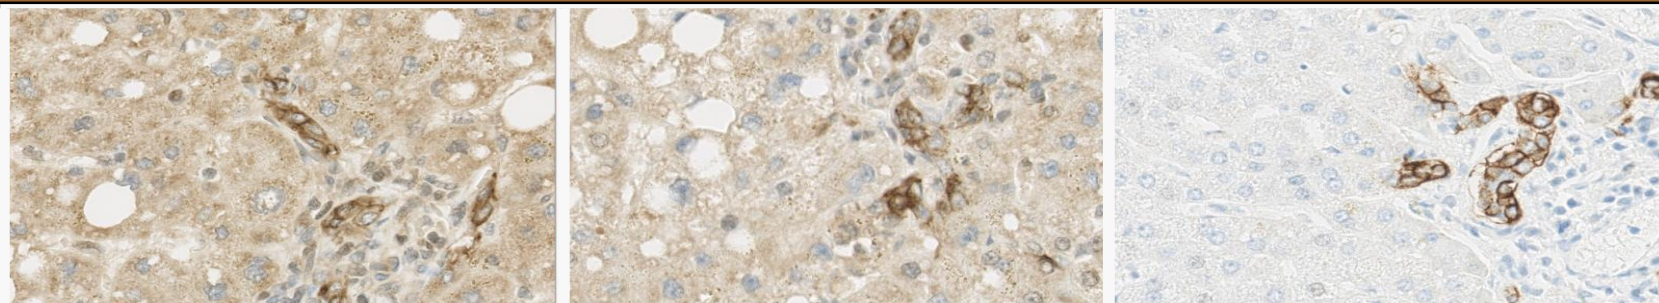

1. Technical calibration – 2. analytical validation

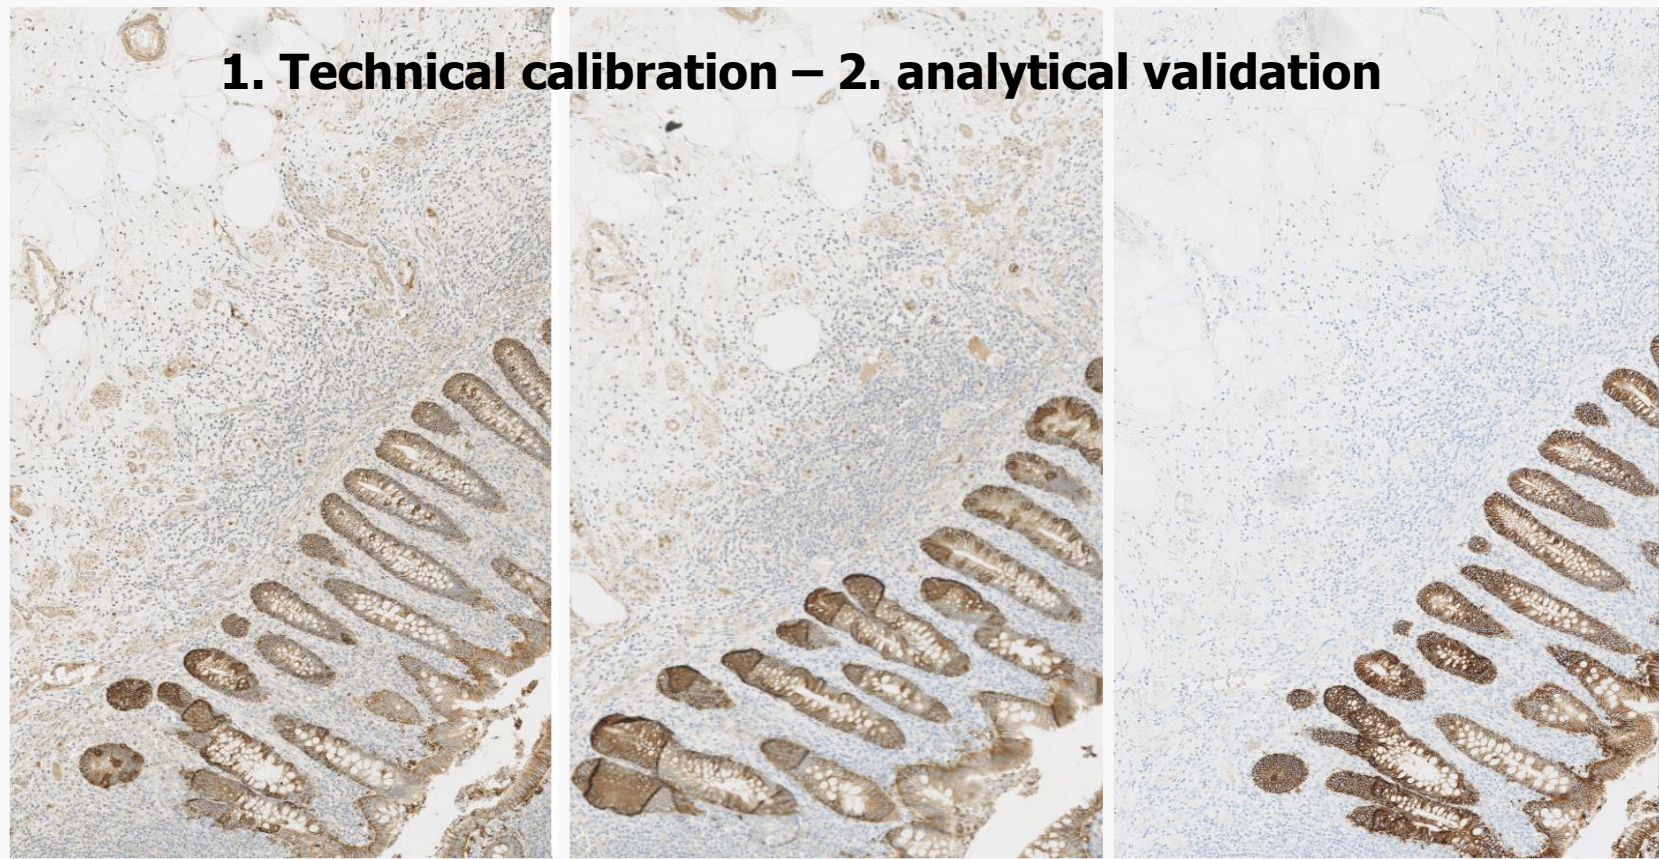

1:100

1:250


1:600

pAb ab71916 – 20 min. RT – HIER 20 min. Low pH – 3-step pol.



IHC – Biomarker controls

Abcam ab 71916: **1:600**, HIER TRS pH 6.1, 3-step polymer


Glioma

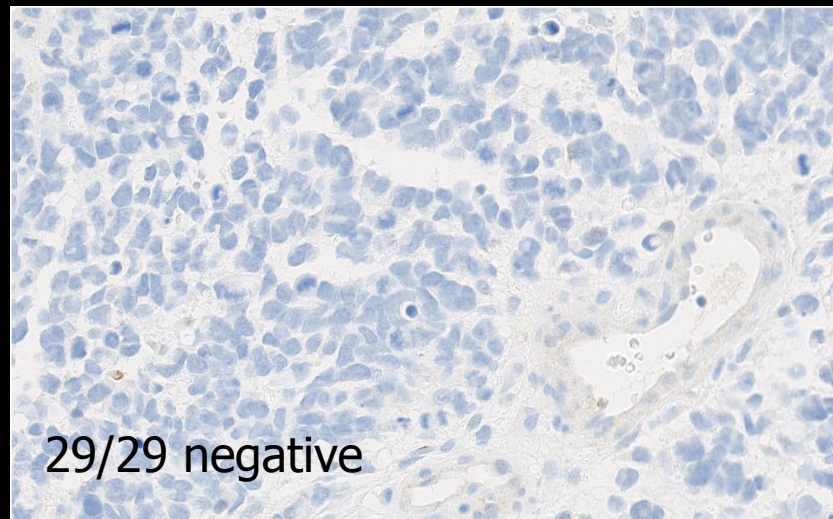

Kidney

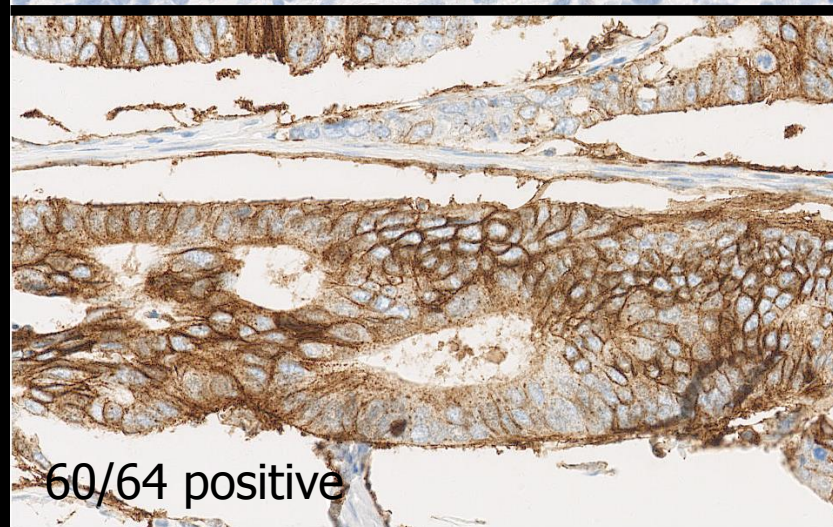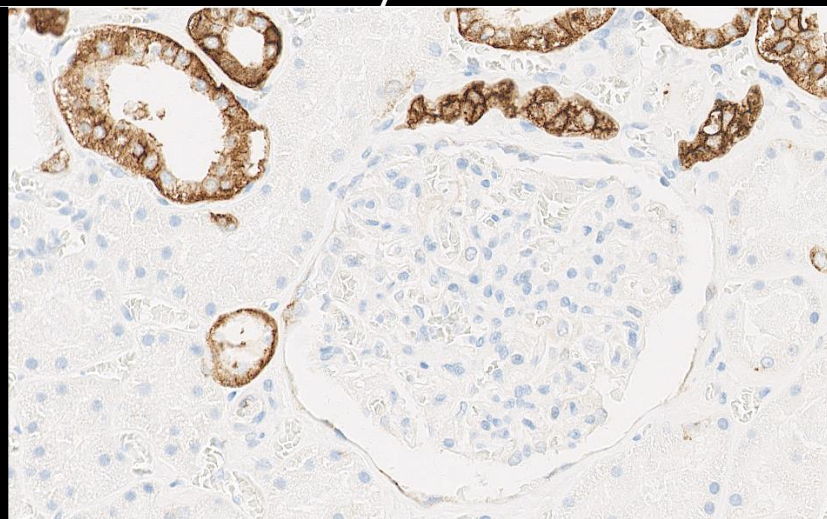

Colon ad. carc.

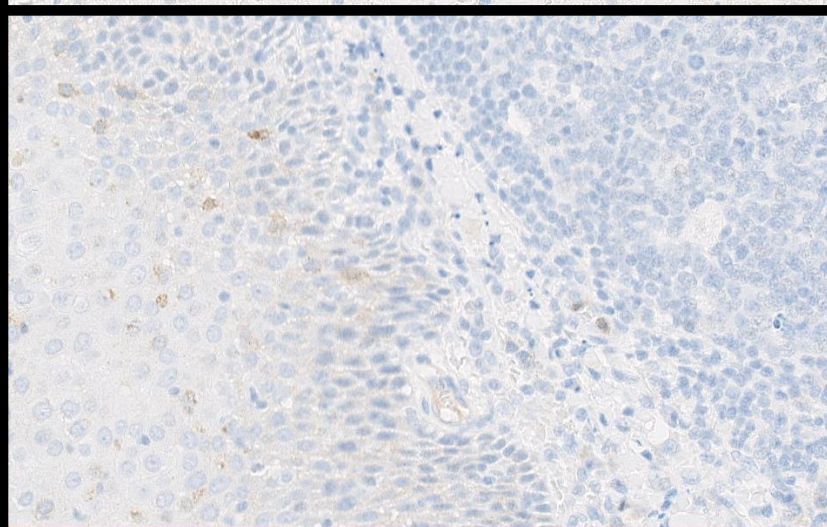

Tonsil

Methods:

Int J Clin Exp Pathol 2014;7(11):7907-7914
www.ijcep.com /ISSN:1936-2625/IJCEP0002589

Polyclonal

- HIER Citr
- 1:100, 16
- 3-step po

Positive (ti

Negative (

Original Article

Overexpression of EpCAM and Trop2 in pituitary adenomas

Xin Chen^{1,2*}, Bo Pang^{2*}, Yu Liang^{1,2}, Shang-Chen Xu¹, Tao Xin¹, Hai-Tao Fan¹, Yan-Bing Yu³, Qi Pang¹

¹Department of Neurosurgery, Shandong Provincial Hospital Affiliated to Shandong University, Jinan 250021, P. R. China; ²Shandong University School of Medicine, Jinan 250012, P. R. China; ³Department of Neurosurgery, China-Japan Friendship Hospital, Beijing 100029, P. R. China. *Equal contributors.

Received September 17, 2014; Accepted November 1, 2014; Epub October 15, 2014; Published November 1, 2014

All data based on inadequately calibrated protocol, inadequate controls and thus false positive results

J Neurooncol (2014) 119:39–47
DOI 10.1007/s11060-014-1459-5

LABORATORY INVESTIGATION

The overexpression of Epithelial cell adhesion molecule (EpCAM) in glioma

Xin Chen · Wei-Yuan Ma · Shang-Chen Xu · Yu Liang · Yi-Bing Fu ·
Bo Pang · Tao Xin · Hai-Tao Fan · Rui Zhang · Jian-Gang Luo ·
Wen-Qing Kang · Min Wang · Qi Pang

Main aim with IHC controls

To confirm that the IHC result can be trusted and subsequently used to analyze our specimen.

Guidance to analytical sensitivity
Guidance to analytical specificity



3 main practical areas of controls in diagnostic IHC


1. Calibration of IHC assay and identification of best practice protocol – clone, titre, retrieval etc
"Evaluation of the robustness – impact on pre-analytics.
2. Analytical validation – diagnostic potential
Sensitivity / specificity.
3. IHC performance controls – to monitor that the established level of detection is obtained in each test performed in daily practice – method transfer.

Virtually always; external tissue control

- **Reagent** and **tissue** controls are necessary for the validation of immunohistochemical staining results.
- **Reagent controls** typically used to validate specificity of the primary and secondary antibodies – to show that the antibody-antigen reaction is due to expression of the target of interest.
 - Often referred as negative controls
- **Tissue controls** typically used to show that the IHC staining was successful and capable to demonstrate the target of interest
 - Often referred as positive controls


- **Reagent** and tissue controls are necessary for the validation of immunohistochemical staining results.
- **Reagent control of the primary antibody is crucial for the producer to validate specificity and can include**
 - Primary ab tested on knock-out mice
 - Primary ab tested on cell lines +/- antigen of interest
 - Primary ab tested by western blotting
 - Primary ab tested by antigen absorbtion
 - Primary ab tested on wide range of tissues/neoplasias

To secure specificity of primary ab -
Both by launch and new ab lots.

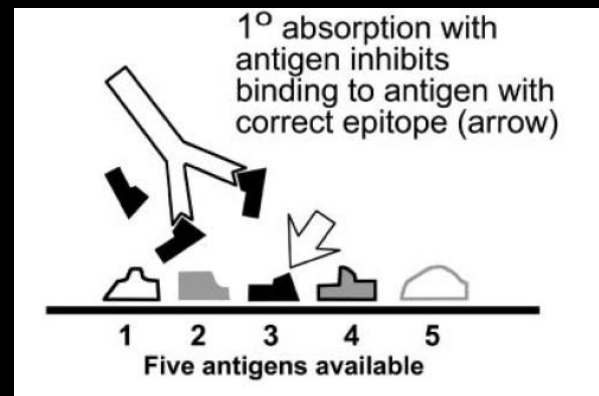


- **Reagent** and tissue controls are necessary for the validation of immunohistochemical staining results.
- Negative reagent control is for the laboratories of limited use and “impossible” to perform correctly.
 - **Primary ab control – *negative reagent control***
 - Each primary ab must have its own negative control serum, and thus all the IHC slides performed will be doubled

- Reagent control is of limited use and impossible to perform correctly.
 - e.g. mAb clone PS1 CD3, IgG1a, Ig. conc 80 ug. Primary Ab is diluted 1:100
 - Neg control mouse serum, IgG1a, Ig conc 120 ug. Must be diluted 1:150 to match CD3

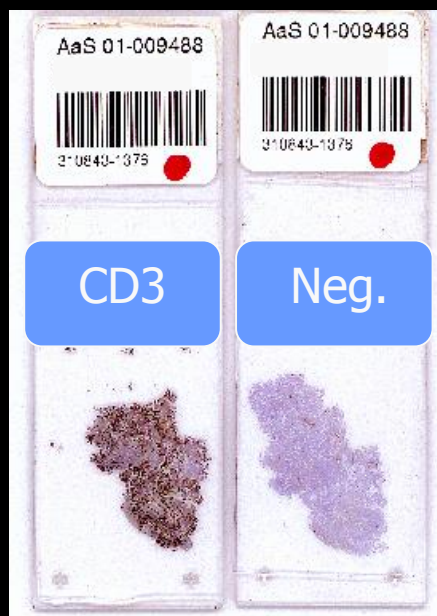

By a work-load of 25.000 slides = 50.000 slides.

By a price pr test of 6 euro the total increase will be 150.000 euro...

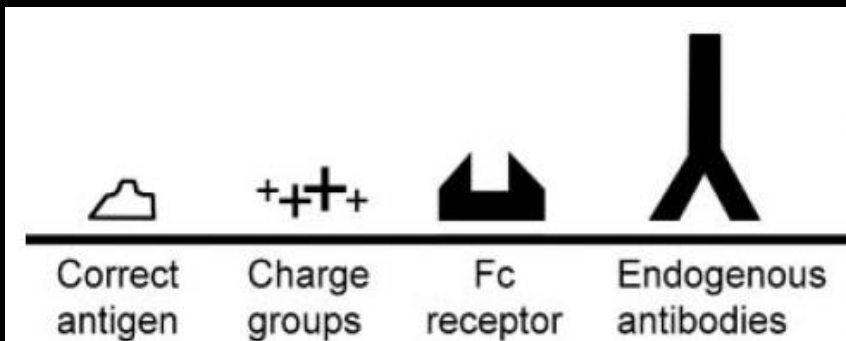

- **Reagent** and tissue controls are necessary for the validation of immunohistochemical staining results.
- Negative reagent control is for the laboratories of limited use and “impossible” to perform correctly.
 - **Secondary ab control – *negative reagent control***
 - The primary ab is substituted by e.g. diluent in order to monitor binding of the detection system to the tissue. In principle each of all retrieval methods applied in a diagnostic case must have its own negative diluent control.
 - Question – what is the value ?


- **Reagent** and tissue controls are necessary for the validation of immunohistochemical staining results.
- Negative reagent control is for the laboratories of limited use and “impossible” to perform correctly.
 - Primary ab control – negative reagent control
 - *Ig subtype precisely calibrated*
 - Secondary ab control – negative reagent control
 - *Diluent or buffer*

WILL NOT EXPOSE IF WRONG, POOR CALIBRATED
OR CONTAMINATED PRIMARY AB WAS APPLIED!!!!!



IHC – Biomarker controls

Study: Abcam ab 71916: 1:100, HIER TRS pH 6.1, 3-step polymer


Glioma

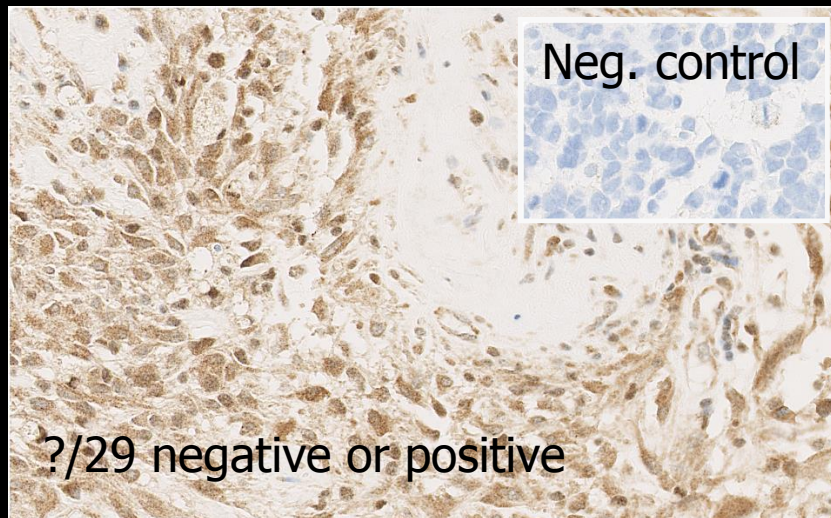

Kidney

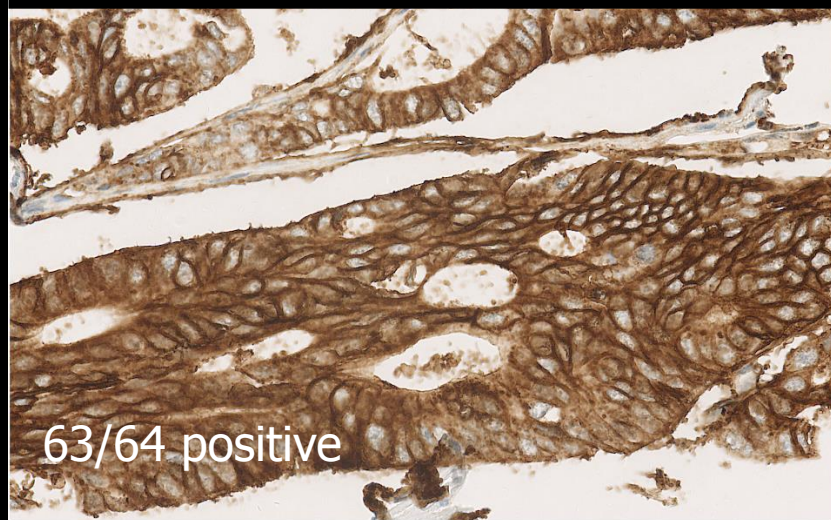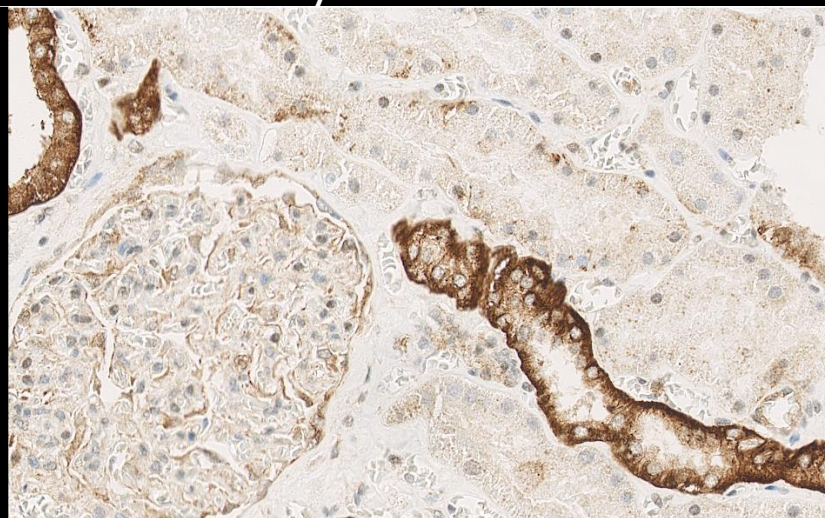


Colon ad. carc.

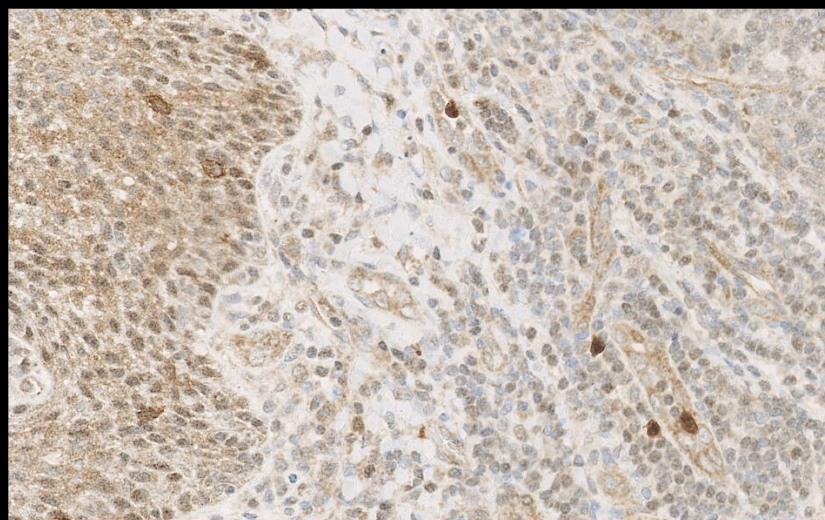


Tonsil


IHC – Biomarker controls

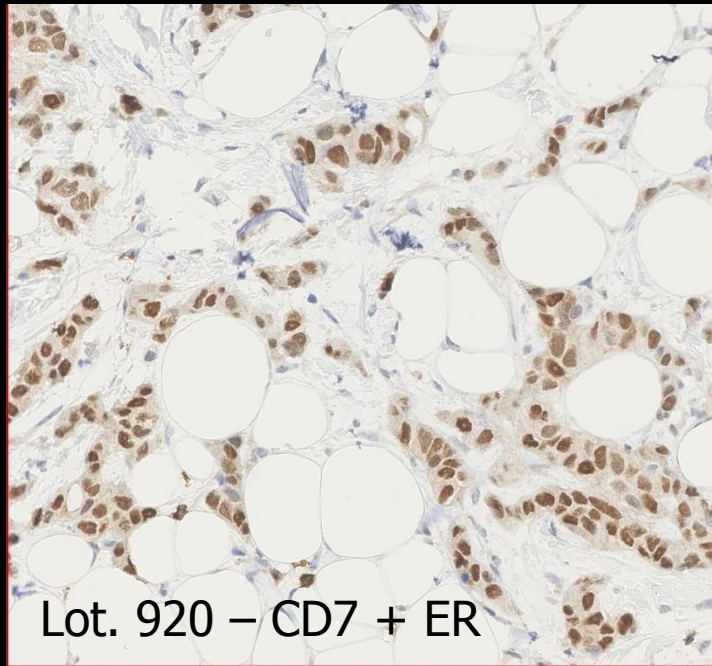


Lot. 920 – CD7 + ER

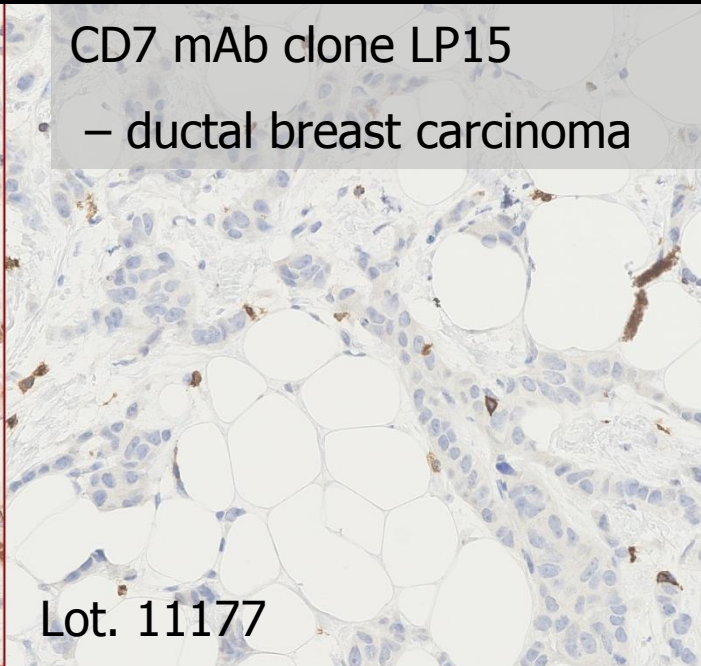

Lot. 11177

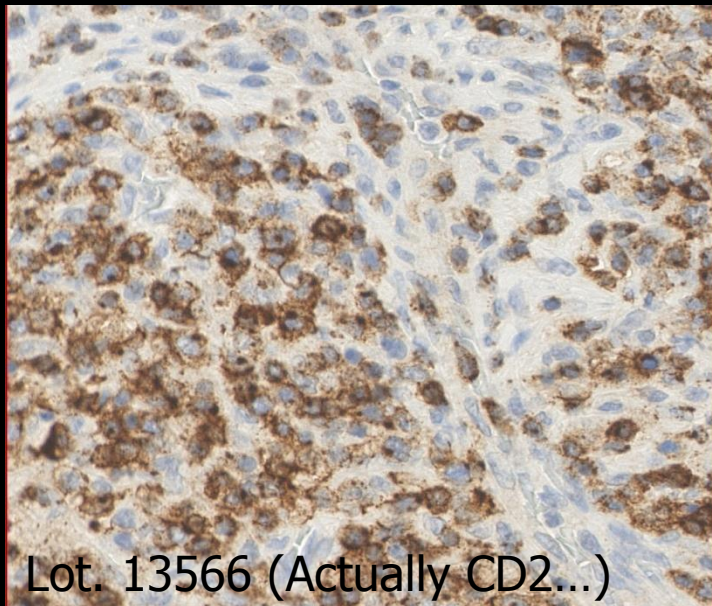

Lot. 13566 (Actually CD2...)

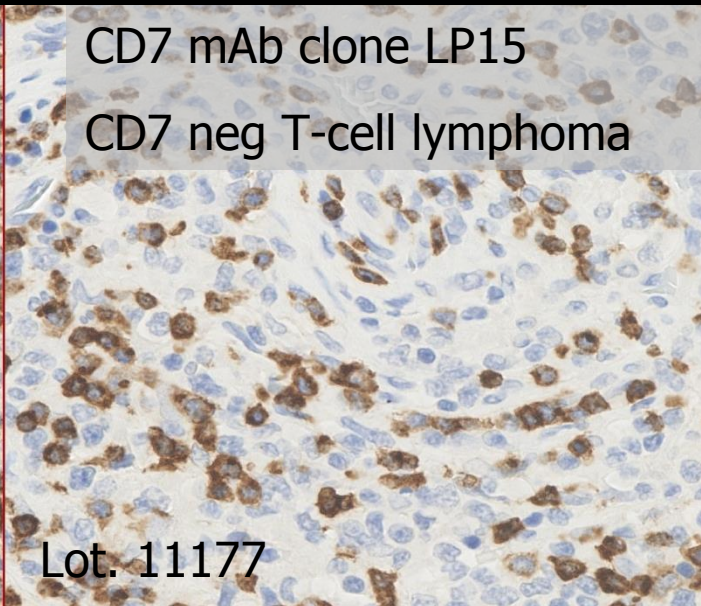

Lot. 11177

CD7 mAb clone LP15

– ductal breast carcinoma

CD7 mAb clone LP15

CD7 neg T-cell lymphoma

FP staining reactions

Not identified by negative reagent controls

The antibody giving the FP would be substituted by control serum and no staining seen giving a "false security"

BSAP rmAb clone SP34
– NordiQC run 41, 2014

FP staining reactions
Not identified by negative reagent controls or
other controls by 3 vendors and 5 laboratories



Fig.4a (X200)

Optimal BSAP staining of the appendix using same protocol as in Figs. 1a - 3a. The peripheral B-cells show a strong nuclear staining reaction, while the epithelial cells are negative.



Fig. 4b (X200)

Aberrant BSAP staining of the appendix. In addition to the expected staining result for BSAP of the B-cells, the epithelial cells display a staining reaction corresponding to CK20. This aberrant staining result was frequently seen, when the rmAb clone SP34 was used as a concentrate and most likely caused by a contamination of the raw material of the clone. The staining reaction was seen in products from all companies providing the clone as a concentrate (see table 1).

IHC – Biomarker controls

Negative reagent control (diluent):

Must: 1. Biotin based detection systems
2. Certain class II / III assays


Can: 1. Pigmented tumours
2. Frozen sections
3. (No internal or external negative tissue structures)

Standardization of Negative Controls in Diagnostic Immunohistochemistry: Recommendations From the International Ad Hoc Expert Panel

Emina E. Torlakovic, MD, PhD,*†‡ Glenn Francis, MBBS, FRCPA, MBA, FFSc (RCPA),§¶
John Garratt, RT,†‡§ Blake Gilks, MD, FRCPC,†‡** Elizabeth Hyjek, MD, PhD,*
Merdol Ibrahim, PhD,†† Rodney Miller, MD,‡‡ Søren Nielsen, HT, CT,§§||
Eugen B. Petcu, MD, PhD,§ Paul E. Swanson, MD,¶¶ Clive R. Taylor, MD, PhD,###
and Mogens Vyberg, MD§§||



TABLE 2. Recommendations for Use of Negative Controls in Diagnostic Immunohistochemistry

Type of Control	CAP-ACP Clinical Use IHC Test Class I	CAP-ACP Clinical Use Class II Tests		Comments
	FDA IHC Device Class I	FDA IHC Device Class II	FDA IHC Device Class III	
Negative reagent control (NRC) NRC-primAb—replace primary Ab with “nonspecific” Ig	Recommended for initial antibody validation, and for use with avidin-biotin detection Not recommended for routine daily use of validated protocol using polymer-based detection Can be ordered by pathologist in specific situations (see text)	Recommended as per published guidelines When no guidelines exist, the NRC antibody control is recommended where results may dictate definitive treatment (ie, ER, PR), and are not confirmed by other aspects of pathology testing	Use negative reagent controls as per approved guidelines	When panels of several antibodies are used on serial sections, negative staining elements in the different sections serve as a negative reagent controls, obviating the need for a separate negative reagent control in most instances of class I testing Also, pathologists’ interpretation of IHC-SE determines if NRC-primAb is required May require multiple controls if several different retrieval methods are in use May require multiple controls for different components of detection system and if different retrieval methods are in use
NRC-detSys (supplementary negative controls)		Use where unexpected staining is observed in the NRC antibody negative control slide (Table 1)		
Negative tissue control (NTC) Internal NTC—evaluate tissue elements that should be negative in test section of the patient’s sample	Recommended	Recommended	Use negative and positive controls tissue as per approved guidelines	If test section does not include elements that serve as negative controls, then, external tissue control may be informative
External NTC—evaluate tissue elements in control tissue that should be negative	Recommended	Recommended		Control tissues may be derived from archived diagnostic tissue as single sections, or tissue microarrays. Cell lines prepared as cell blocks, if processed in the same way as patient samples can be also be used (see text)

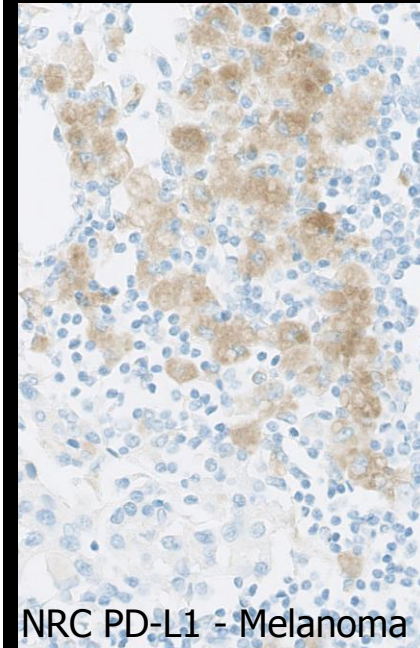

NRC PD-L1 - Melanoma

IHC – Biomarker controls

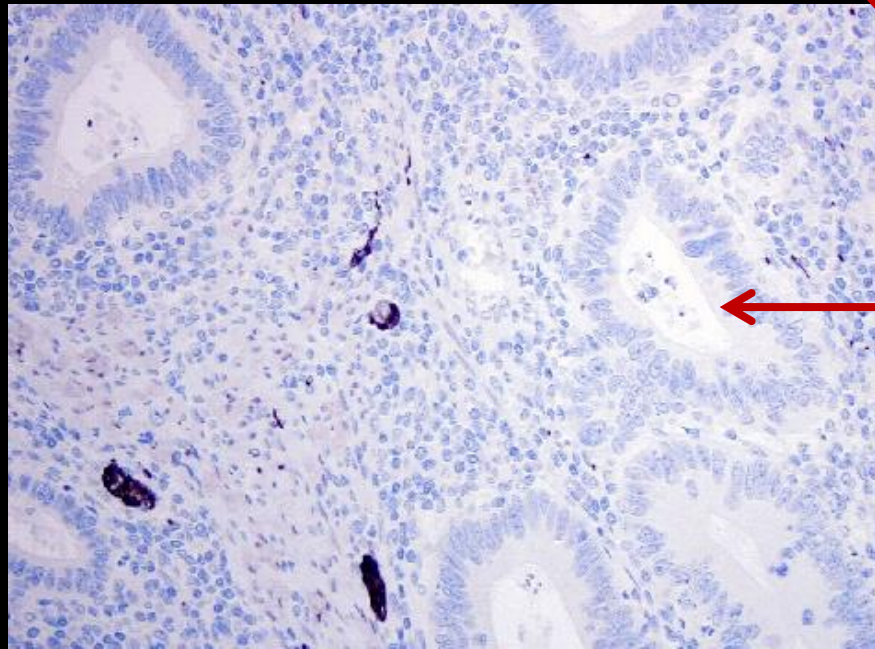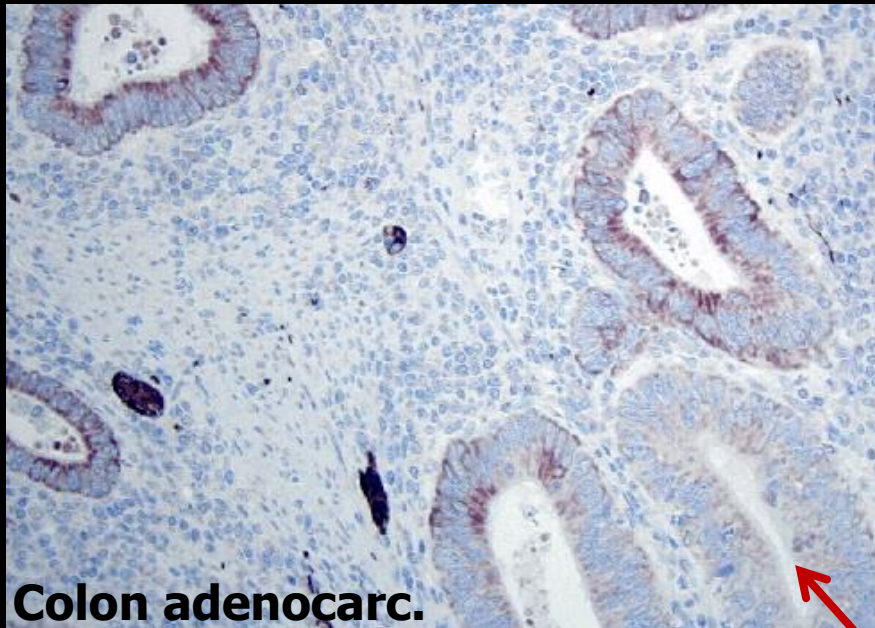

Labelled Steptavidin-Biotin system

Labelled Streptavidin-Biotin system – neg control

Multimer / Polymer based system

Synaptophysin mAb clone 27G12

HIER & biotin-based assays a challenge....
- used by 2-4% of NordiQC participants

- Reagent and **tissue** controls are necessary for the validation of immunohistochemical staining results.
- Tissue controls are the most valuable tool to monitor the specificity and sensitivity for IHC
 - Internal positive and negative tissue control
 - Cells/structures within the patient slide
 - External positive and negative tissue control
 - Slide next to patient slide

- Reagent and **tissue** controls are necessary for the validation of immunohistochemical staining results.
- Tissue controls are the most valuable tool to monitor the specificity and sensitivity for IHC
 - Internal **negative** tissue control
 - Cells / structures to be negative
 - E.g. T-cells for CD19, CD20, CD79a...
 - Mantle zone B-cells for Ki67, Bcl-6...
 - Epithelial cells for CD3, CD5, MUM1,...

Information of primary ab / assay specificity

NordiQC run 35, CD19

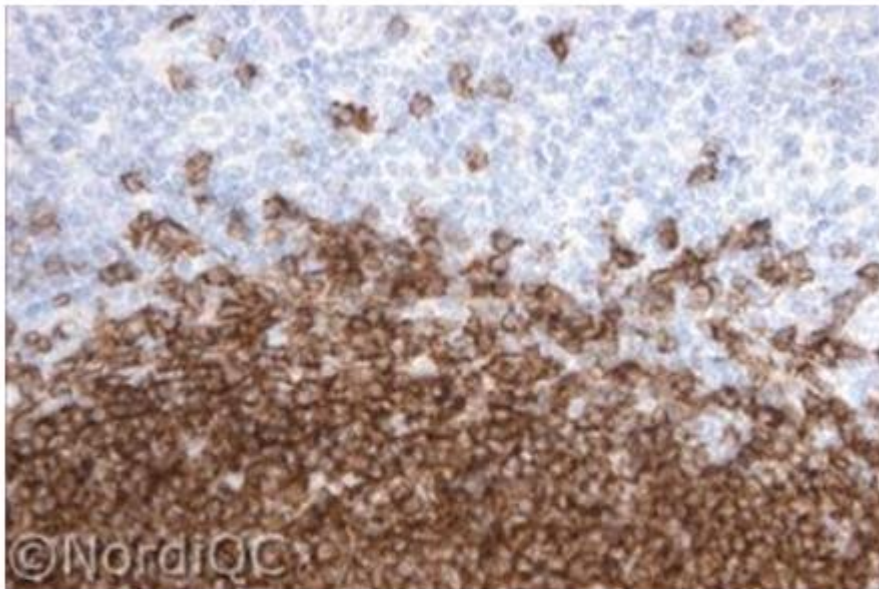


Fig. 1a. Normal tonsil showing an optimal staining for CD19 using the mAb clone LE-CD19 from Dako, diluted 1:50, on the Autostainer platform. HIER was performed using TRS pH 9 (3-in-1) (Dako). A strong and distinct membranous staining reaction is seen in virtually all B-cells. T-cells are negative.

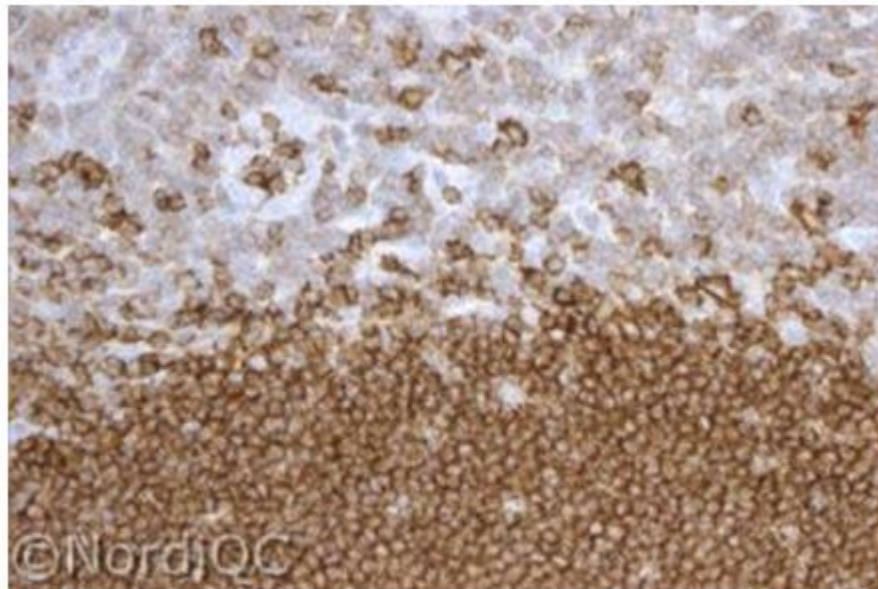


Fig. 1b. Normal tonsil showing an insufficient staining for CD19 using the mAb clone LE-CD19 from Serotec, diluted 1:500, on the Autostainer platform. HIER was performed using Citrate pH 6. In addition to a moderate to strong staining reaction in the normal B-cells (albeit weaker than that seen in Fig 1a), the majority of T-cells shows a false positive staining reaction.


mAb clone LE-CD19

Dako:	B-cells positive, T-cells negative
Serotec:	B-cells positive, T-cells <u>false</u> positive


IHC – Biomarker controls

CD7 mAb clone LP15

– ductal breast carcinoma

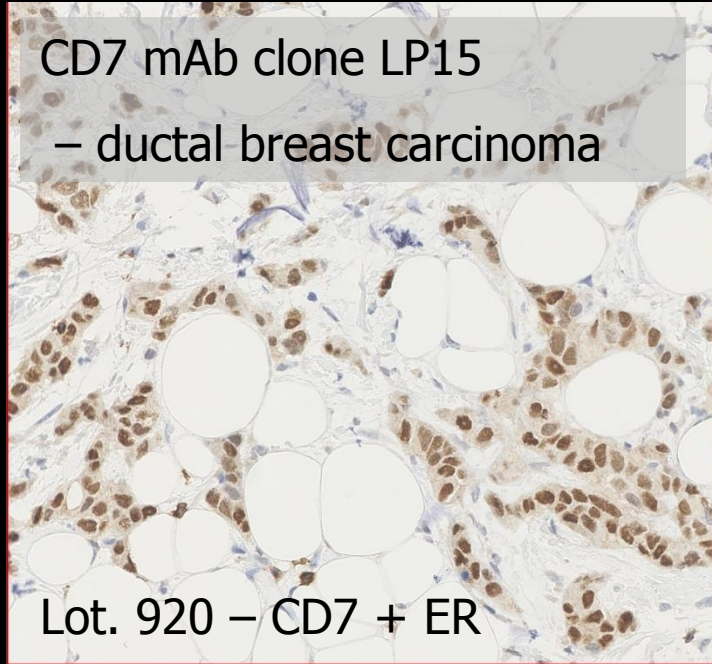

Lot. 920 – CD7 + ER

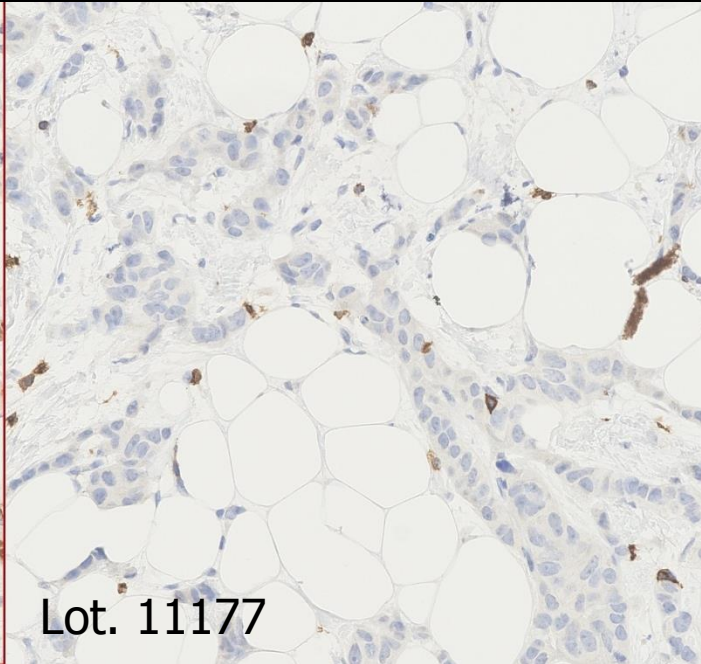

Lot. 11177


FP staining reactions

Not identified by negative reagent controls


The antibody giving the FP would be substituted by control serum and no staining seen giving a "false security"

BSAP rmAb clone SP34


Appendix

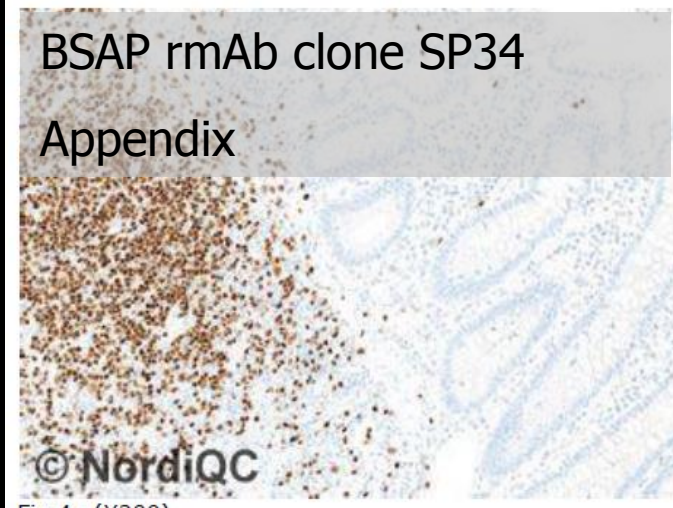


© NordiQC

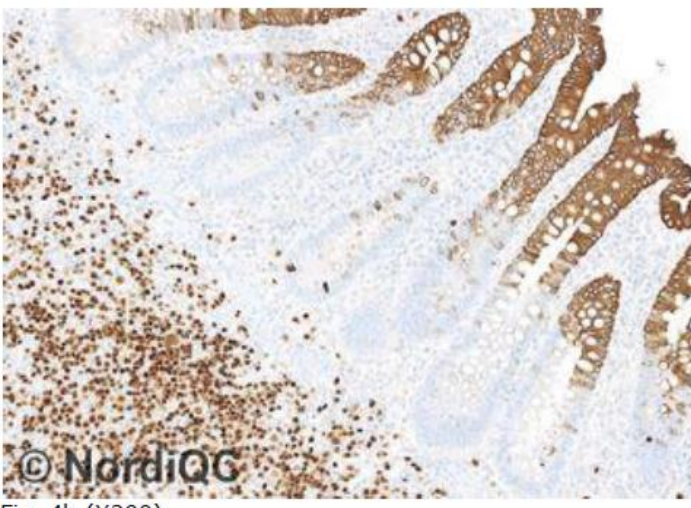


© NordiQC

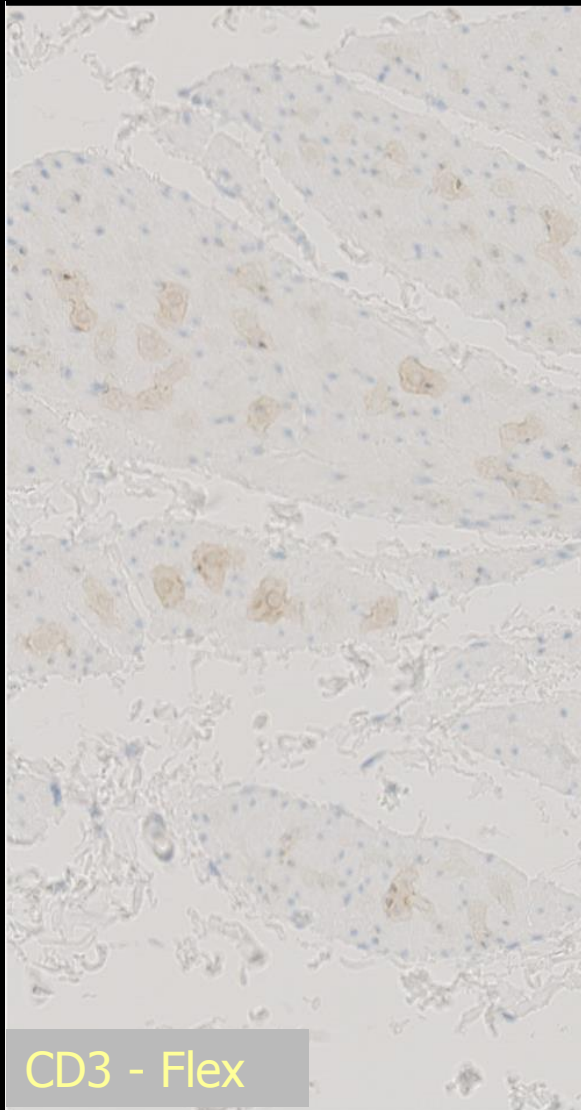

CD3 - Flex

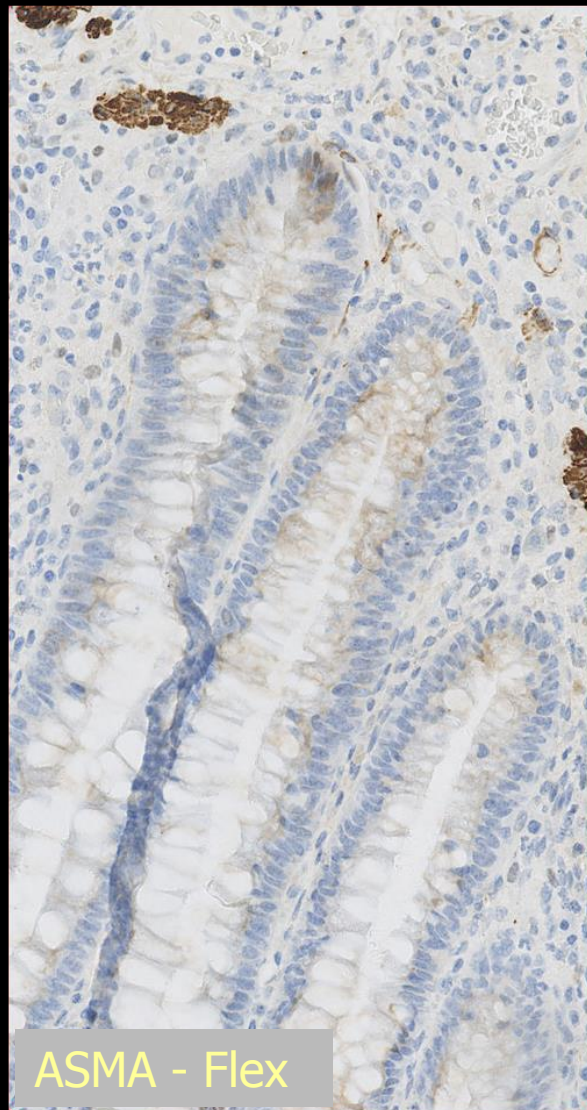

ASMA - Flex

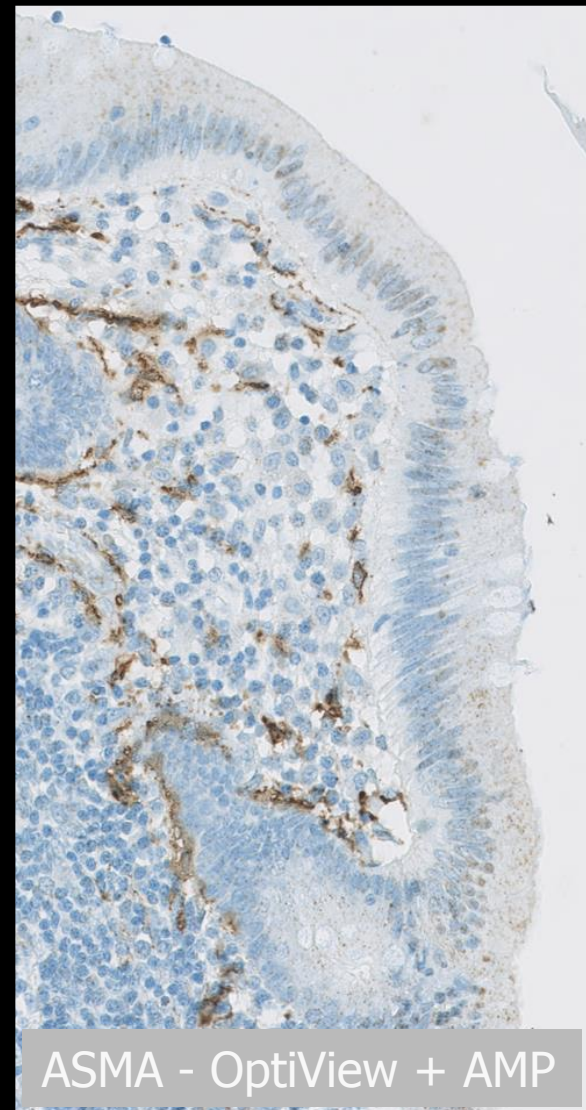

ASMA - OptiView + AMP

Internal structures used as negative tissue control for **polymer**/multimer based detection systems

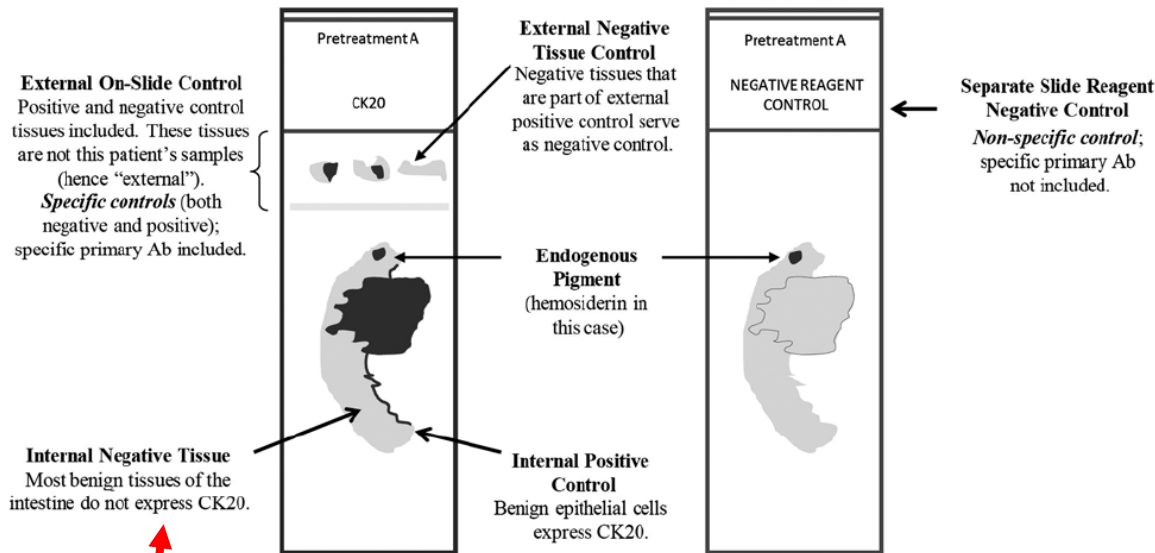


FIGURE 1. “On-slide” external and internal negative tissue controls are illustrated. It is sound practice whenever possible to include cells (or tissue elements) that will serve as negative controls (expected to be nonreactive) when selecting tissue for the positive tissue control. Both internal and external negative on-slide tissues are so-called “specific” negative controls because all are exposed to the specific primary antibody. Separate slide negative controls are generally used for negative reagent controls, where the primary antibody is omitted or an irrelevant primary antibody is used. Note that reagent controls should have identical protocols to the specific immunohistochemistry test, including the same type of pretreatment, as far as is possible.

What about internal positive tissue controls ???

Internal neg tissue control: Identification of false-positive staining reaction of structures known not to express the target antigen.

Limitation: Not all elements will be available to expose a potential false positive result

PAX5.... 3 vendors


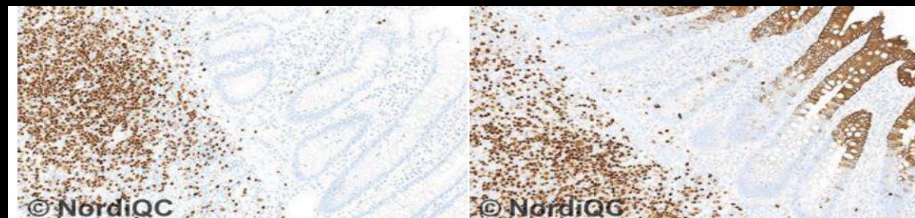


TABLE 2. Examples of IHC Assays Where Preferential Use of Internal Positive Controls Recommended

IHC Assay	Use	Comments
Cytokeratin 5	Demonstration of basal cells in glandular structures of prostate to differentiate between benign (positive) and malignant (negative) glands	Interpretation of the results in the tumor directly depends on clear demonstration of internal positive control Tested sample may be completely negative if no normal tissue is present
Mismatch repair proteins (MLH1, MSH2, PMS2, MSH6)	Absence of expression in the cells of colon or endometrial adenocarcinoma is abnormal; patients referred for molecular testing to rule out Lynch Syndrome	Interpretation of the results in the tumor directly depends on clear demonstration of internal positive control
SMAD4/Dpc4	Ubiquitously expressed tumor suppressor Ag that is inactivated in about 55% of pancreatic adenocarcinomas	Interpretation of the results in the tumor directly depends on clear demonstration of internal positive control
PTEN	Ubiquitously expressed; loss of expression is associated with carcinogenesis, cancer progression, and drug resistance	Interpretation of the results in the tumor directly depends on clear demonstration of internal positive control

Internal positive tissue controls;

Principally ideal as processed identically to patient relevant material evaluated

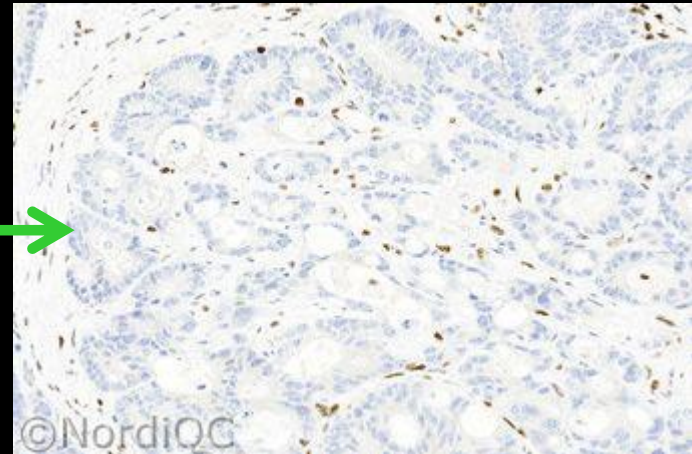

If internal positive control is neg or dubious – test is repeated



IHC – Biomarker controls

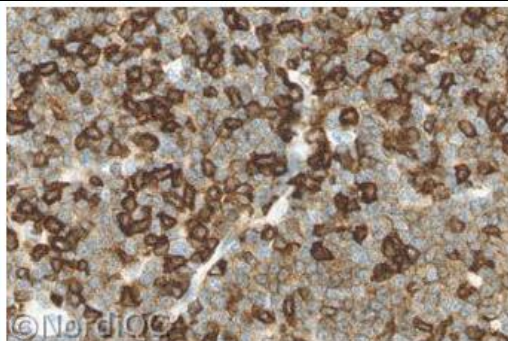


Fig. 4a. Optimal staining for CD5 of the B-CLL no. 5 using same protocol as in Figs. 1a - 4a. The majority of the neoplastic cells show a moderate and distinct staining reaction, while the infiltrating normal T-cells show a strong staining reaction.

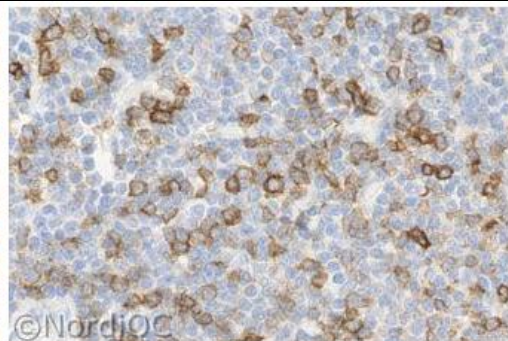


Fig. 4b. Insufficient staining for CD5 of the B-CLL using same protocol as in Figs. 1b - 3b - same field as in Fig. 4a. The neoplastic cells are virtually negative and only the normal T-cells are clearly demonstrated.

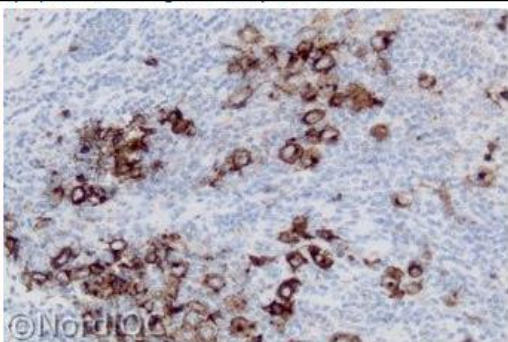


Fig. 2a. Optimal CD15 staining of the Hodgkin lymphoma no. 2 (NS) using same protocol as in Fig. 1a. The Reed-Sternberg and Hodgkin cells show a strong membranous staining and a dot-like positivity.

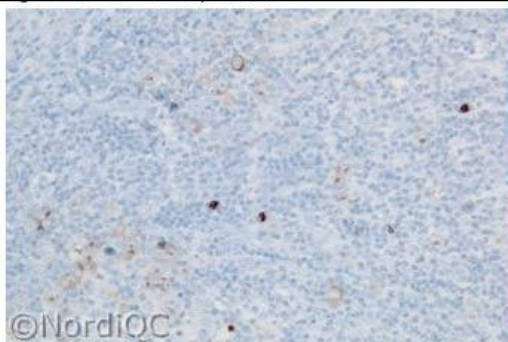


Fig. 2b. CD15 staining of the Hodgkin lymphoma no. 2 (NS) using same protocol as in Fig. 1b. Only few Reed-Sternberg and Hodgkin cells show a weak staining - same field as in Fig. 2a.

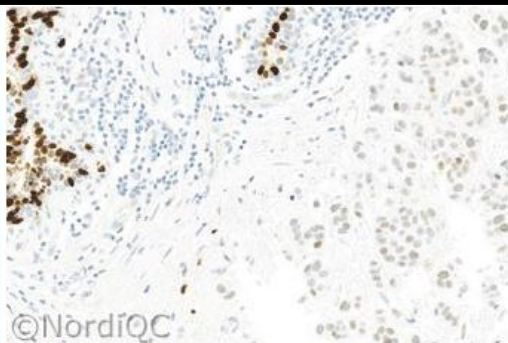


Fig. 3a. Optimal ER staining of the breast ductal carcinoma no. 3 with 60 - 80 % cells positive. A weak but distinct nuclear staining is seen in the appropriate proportion of the neoplastic cells. Same protocol as in Figs. 1a and 2a.


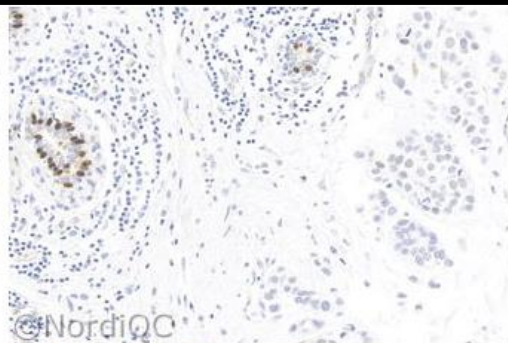


Fig. 3b. Insufficient ER staining of the breast ductal carcinoma no. 3 with 60 - 80 % cells positive using same protocol as in Figs. 1b and 2b - same field as in Fig. 3a. Only dispersed neoplastic cells show an equivocal staining.

Internal positive tissue controls;

In general not applicable as positive controls due to levels of expression may not be relevant for level of test calibration

e.g. CD5, CD15, CD34, CD45, CD56, S100, ER, PR etc

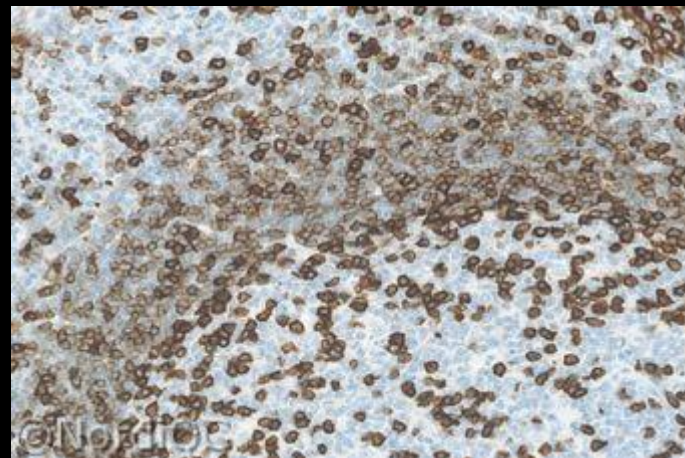

- Reagent and **tissue** controls are necessary for the validation of immunohistochemical staining results.
- **Conclusions – Internal tissue controls**
 - Internal positive tissue control
 - Indicative of "*successful*" IHC result
 - Cannot be recommended as generally reliable for evaluation of appropriate sensitivity
 - Essential for interpretation of MMR
 - Valueable for CK-HMW in prostate
 - Internal negative tissue control
 - Can provide valuable information of specificity of the primary antibody/assay

- Reagent and **tissue** controls are necessary for the validation of immunohistochemical staining results.
- Tissue controls are the most valuable tool to monitor the specificity and sensitivity for IHC
 - **External positive and negative tissue control**
 - Appropriate sensitivity of the IHC assay
 - Appropriate specificity of the IHC assay

The central tool to monitor the technical IHC quality, diagnostic utility and consistency.

Issues to be addressed :

1. Calibration of IHC assay and identification of best practice protocol – clone, titre, retrieval etc
2. "Evaluation of the robustness of the IHC assay – impact on pre-analytics
3. Evaluation of the analytical sensitivity/specificity
4. Identification of IHC performance controls providing information that the established level of detection is obtained in each test performed in daily practice.

Tissue controls are key element

Issues to be addressed :

1. Calibration of IHC assay and identification of best practice protocol – clone, titre, retrieval etc
 - Concentrated formats
 - Full test comprising various titres, retrieval settings, detection systems (+/- different stainer platform)
 - Ready-To-Use formats
 - Confirmatory test primarily using official recommendations and if needed modifications e.g. incubation times, detection system etc

Concentrated antibodies – Aalborg Hospital (app. 200 Abs) – VMS ULTRA

	1:25	1:100	1:400
A	None	None	None
B	Enzyme P1, 4 min	Enzyme P1, 4 min	Enzyme P1, 4 min
C	HIER CC1 pH 8.5*	HIER CC1 pH 8.5	HIER CC1 pH 8.5
D	HIER CC2 pH 6.0**	HIER CC2 pH 6.0	HIER CC2 pH 6.0
<hr/>			
(E)	CC1 + Enzyme P3, 8 min	CC1 + Enzyme P3, 8 min	CC1 + Enzyme P3, 8 min
(F)	Enzyme P3, 8 min + CC1	Enzyme P3, 8 min + CC1	Enzyme P3, 8 min + CC1

*HIER time 48 min. at 99°C, ** HIER time 32 min. at 99°C

32 min in primary Ab, OptiView DAB, Ventana BenchMark Ultra

Protocol A: 2 %

Protocol B: 3 %

Protocol C: 90 %

Protocol E: 3 %

Protocol F: 1 %


Others : 2 % (E.g. prolonged HIER, prolonged proteolysis, amp. Kit....)

Ready-To-Use – VMS ULTRA

RTU

Typical protocol:

A: HIER in CC1 standard (64 min.), 16 min. Incubation time in primary Ab and UltraView-DAB

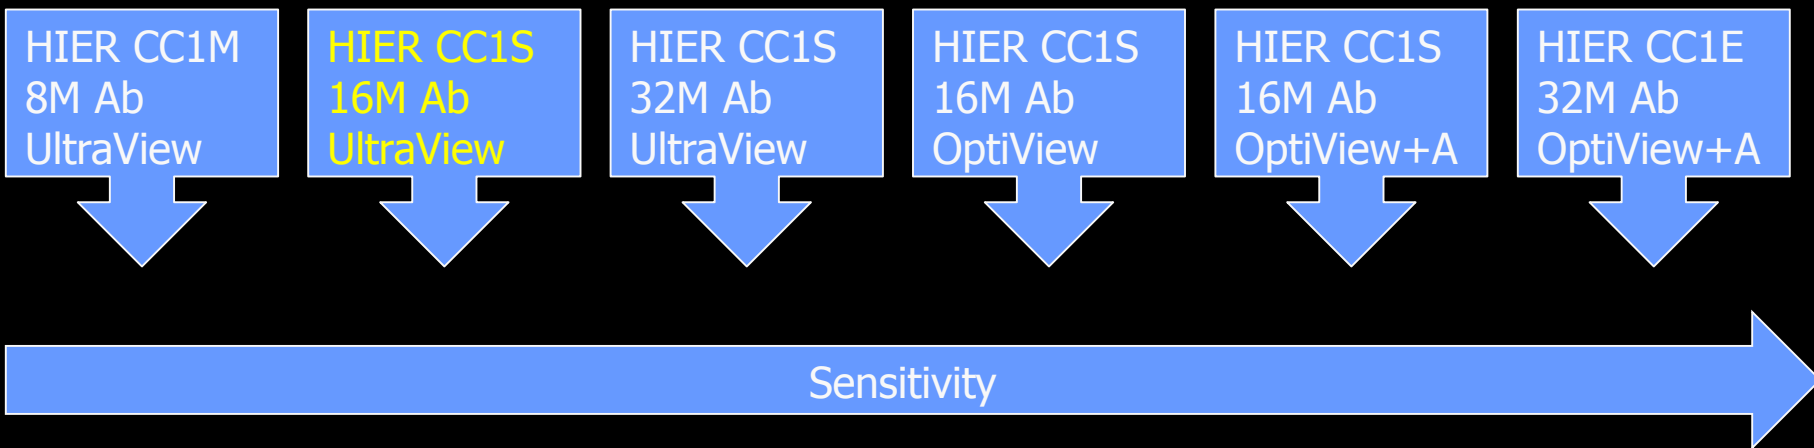

Issues to be addressed :

1. Calibration of IHC assay and identification of best practice protocol – clone, titre, retrieval etc
2. "Evaluation of the robustness of the IHC assay – impact on pre-analytics
3. Evaluation of the analytical sensitivity/specificity
4. Identification of most robust controls providing information that the established level of detection is obtained in each test performed in daily practice.

Tissue controls are key element

Technical test array



1. Calibration
2. Robustness

Appendix	Kidney	Thyroid	
Ton 6h	Ton 24h	Ton 72h	Ton 168h
Liver 6h	Liver 24h	Liver 72h	Lung
Kidney	Brain	Pancreas	Placenta
Testis	Prostate	Esophagus	Ton 24h + decalc.



Protocol set-up: used as primary material for the calibration of 130 of 195 routine diagnostic markers, Aalborg University Hospital

IHC – Biomarker controls



1:100

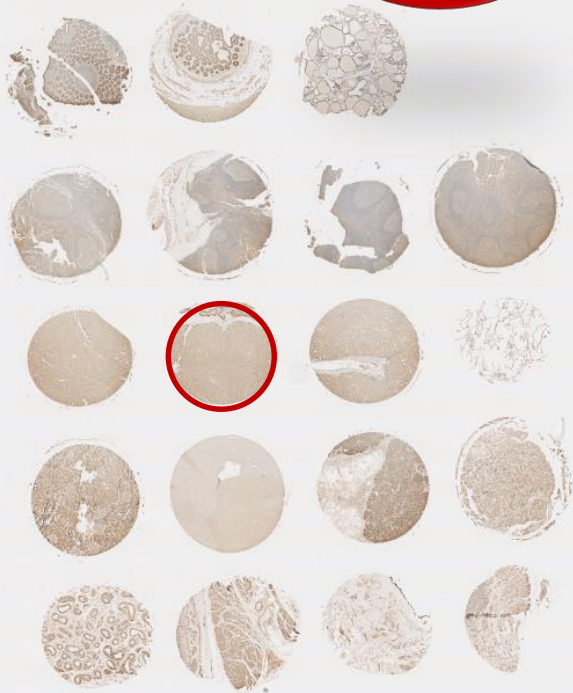

1:250

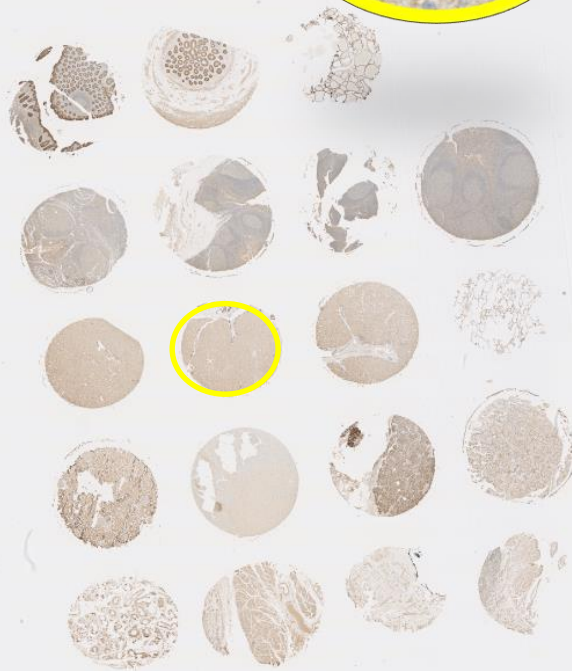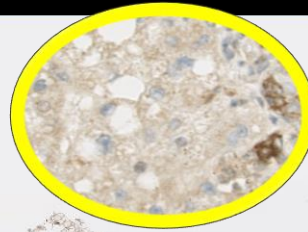

1:600

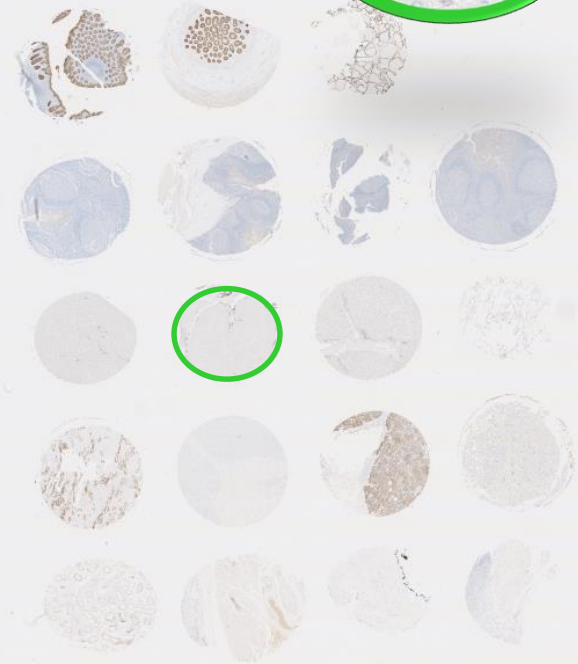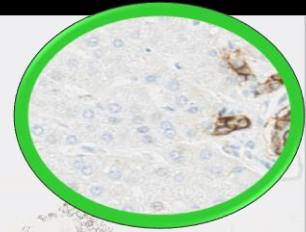

EPCAM calibration

Tissue cores are used to identify best practice protocol providing highest signal-to-noise ratio for qualitative IHC markers




IHC – Biomarker controls

Photos by Ole Nielsen

Technical test array

1. Calibration
2. Robustness

CD105, SNH6

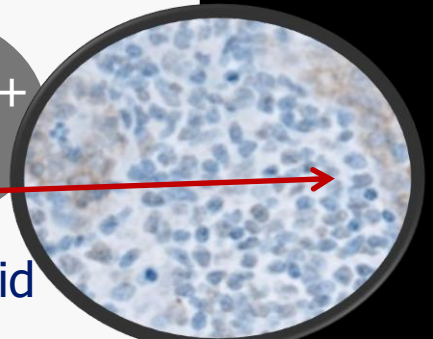
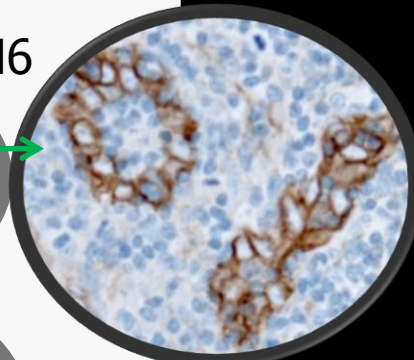
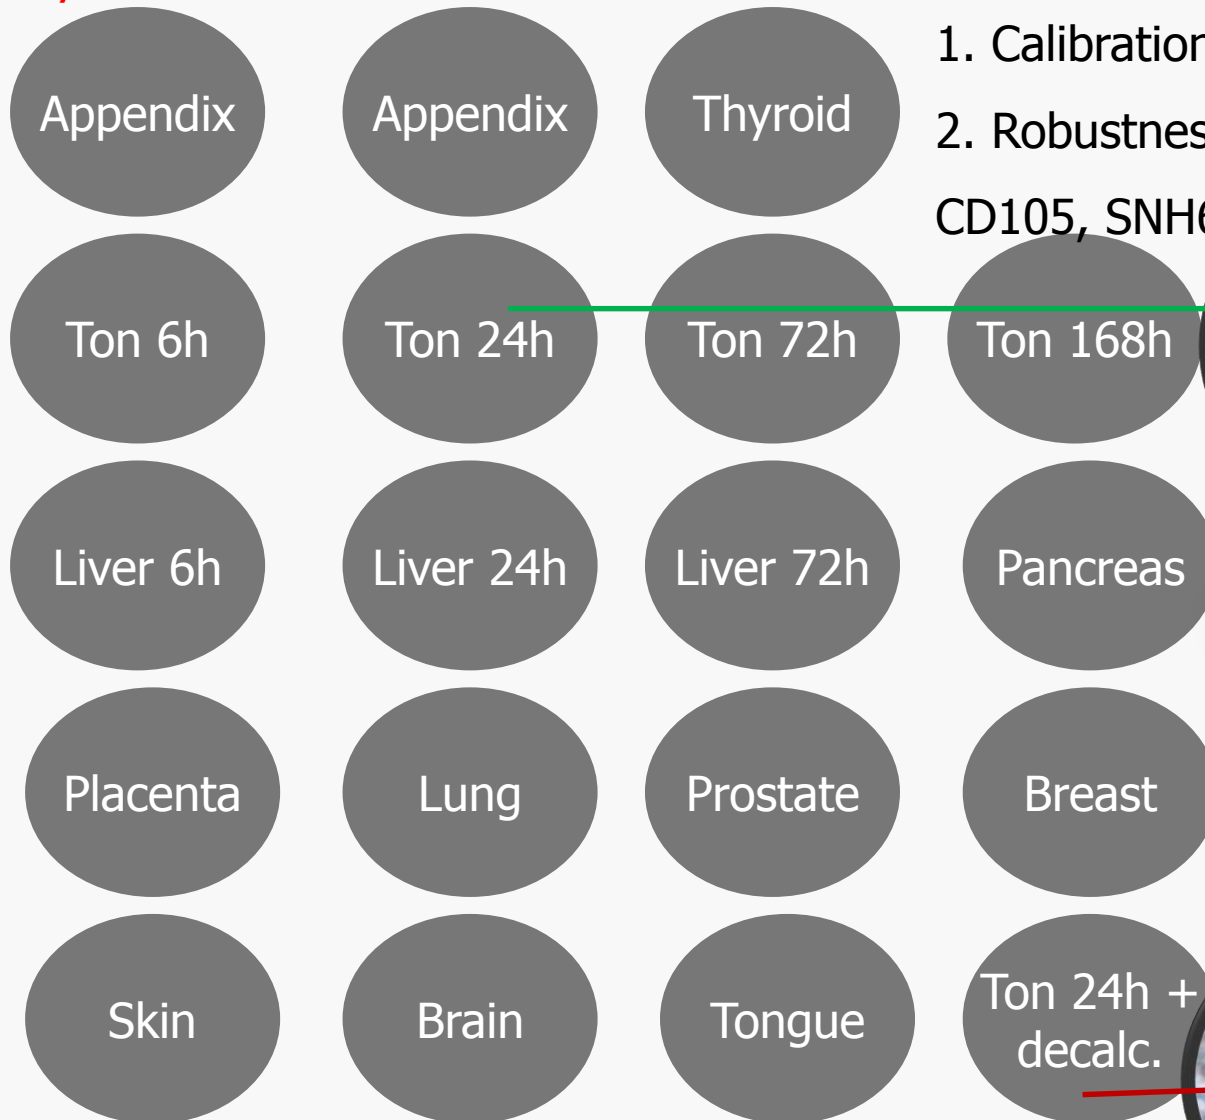


Protocol set-up:

Formic acid

IHC – Biomarker controls

CD52, clone YTH34.5 (Campath)

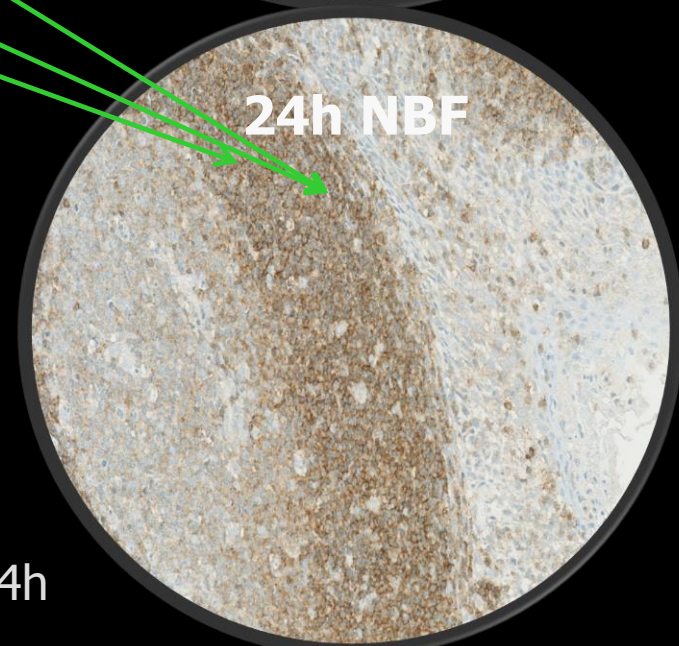
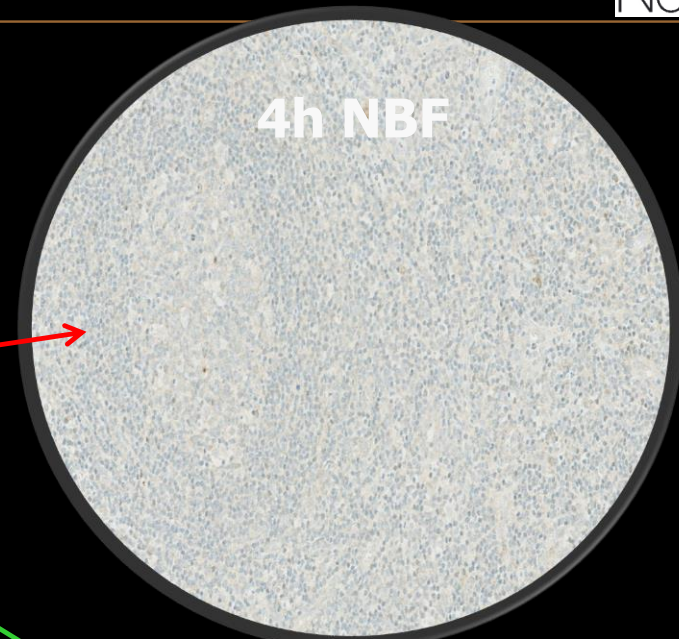
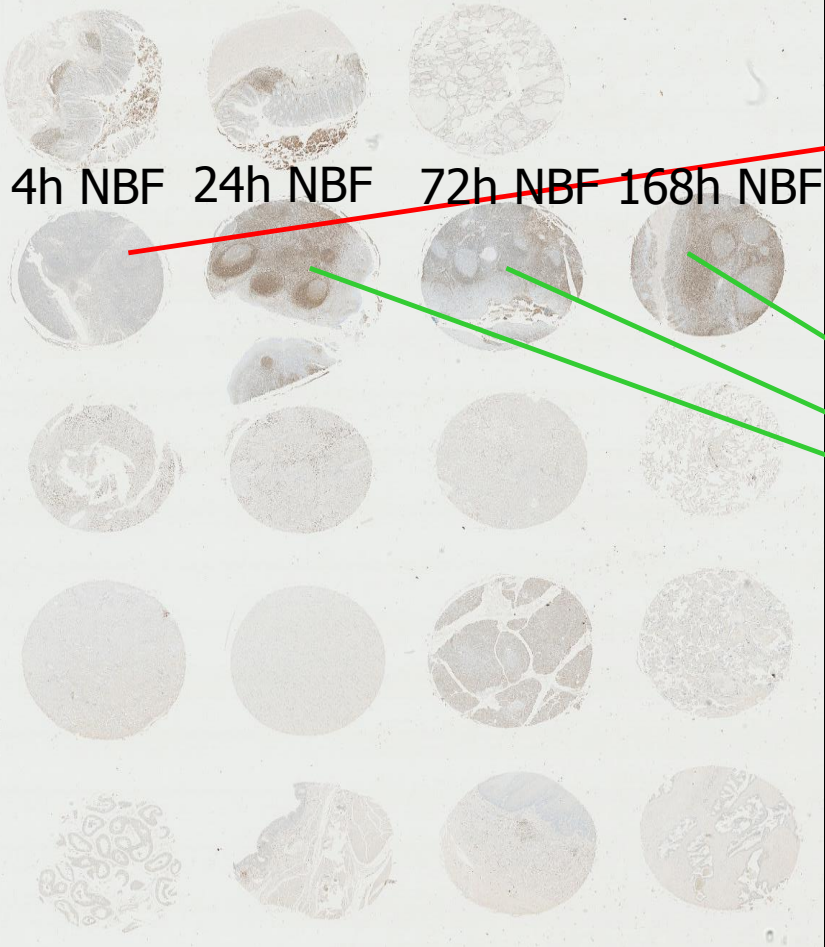


1. Influenced by fixation time – reduced in $<24h$
2. IHC protocol, 3. Control; Tonsil – cave if no B-cells stained, interpret with caution

IHC – Biomarker controls

Anti-CD45 test:

Protocol set-up:

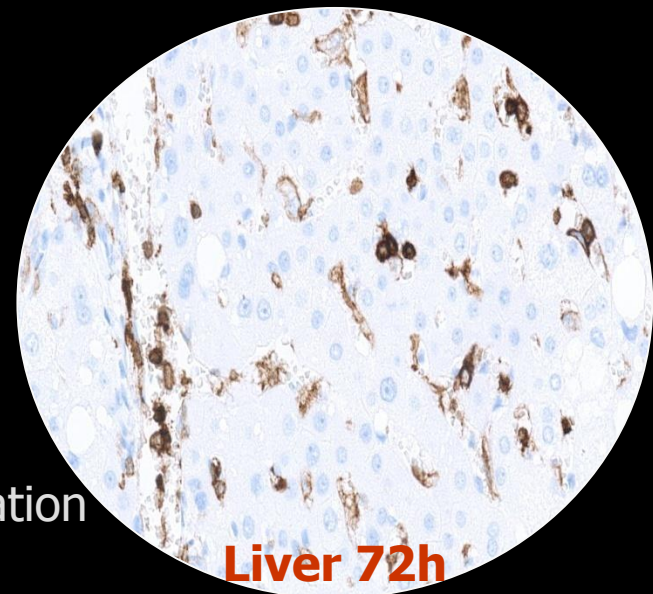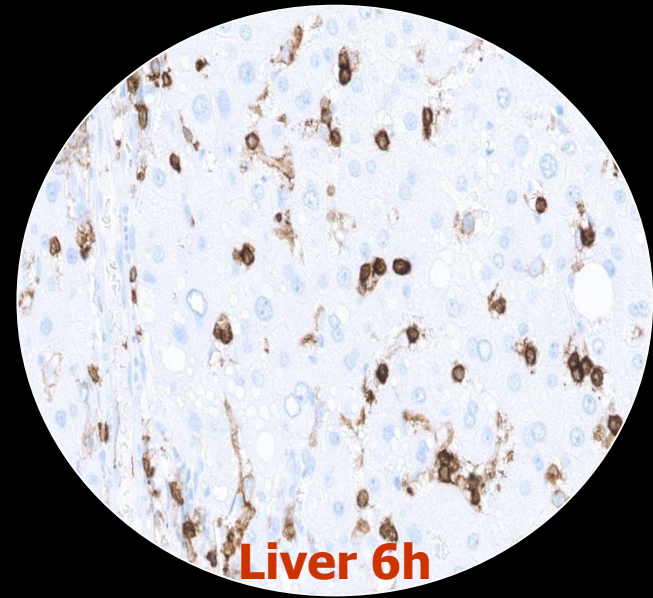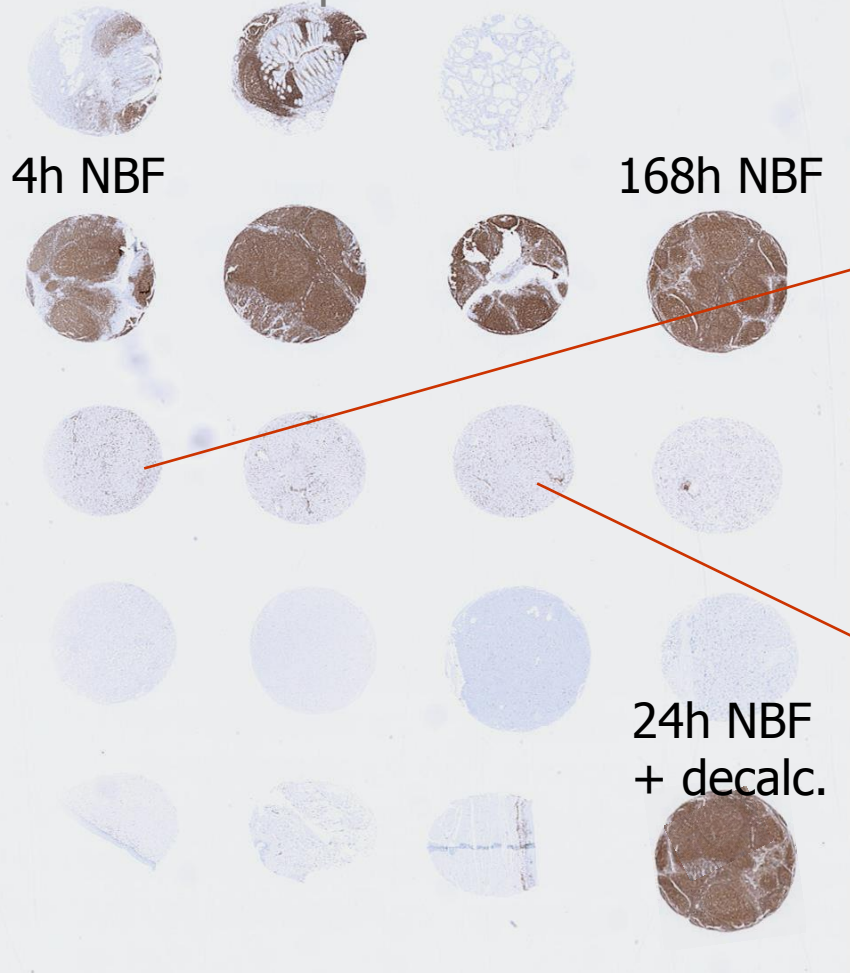




1. Not NBF dependent or influenced by decalcification
2. Liver as control, 3. IHC protocol

IHC test: Fit for purpose –












All IHC tests both laboratory developed assays and RTU systems must be calibrated for the diagnostic use

E.g. IHC assay for CD45 (LCA)

Purpose	Diagnostic utility	Tool	Application
To demonstrate CD45 in bone marrow derived cells / haematolymphoid cells	IHC for CD45 has been shown to be very specific and sensitive as a lineage marker in CUP	To be used in an IHC panel with other markers – e.g. S100, VIM, CK Pan	Identification of a reliable IHC protocol and interpretation guidelines for the pathologist
Diagnostic relevant	Diagnostic validity	Technically possible	Diagnostic possible

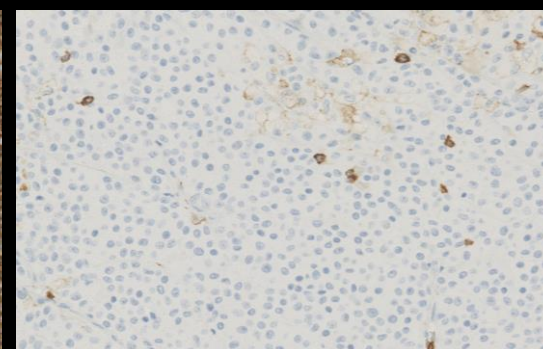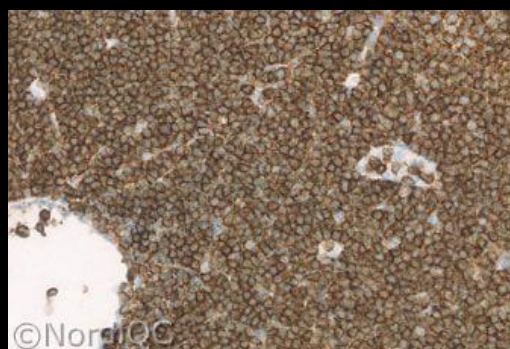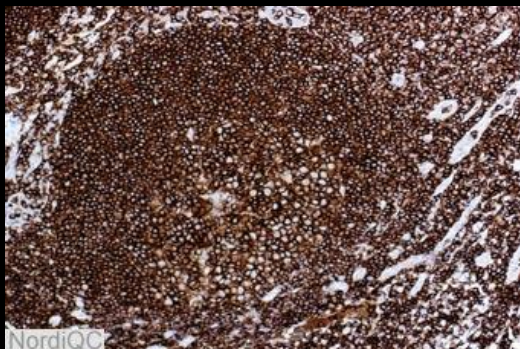

IHC – Biomarker controls

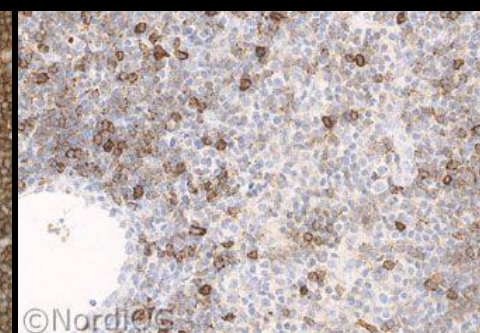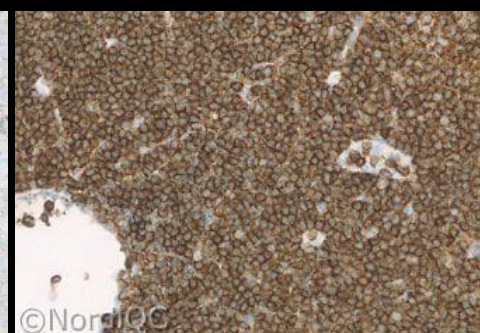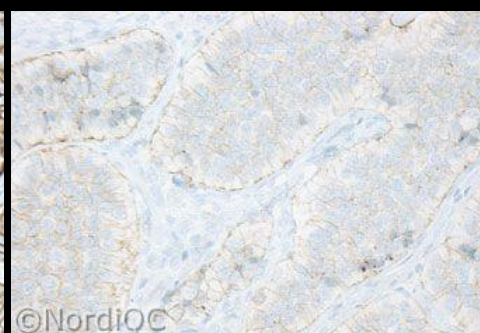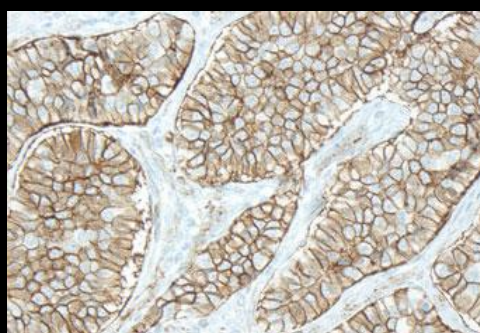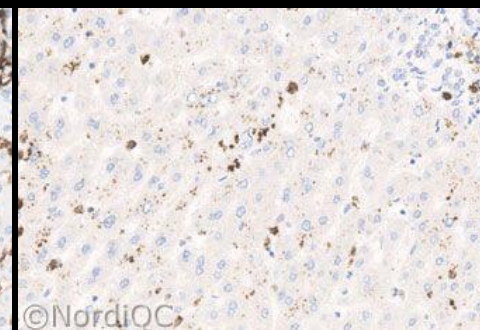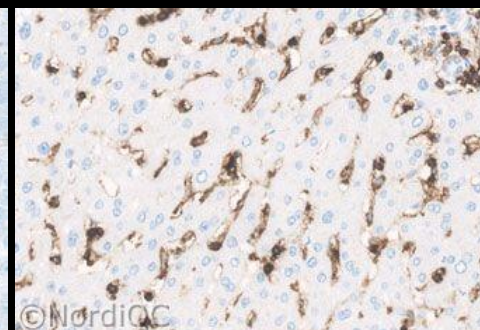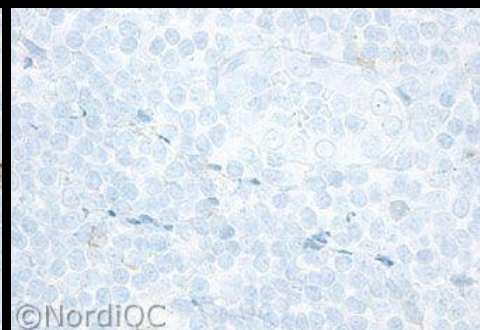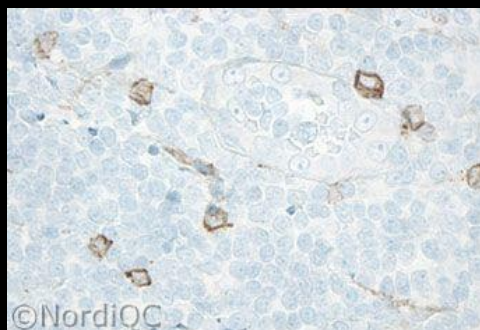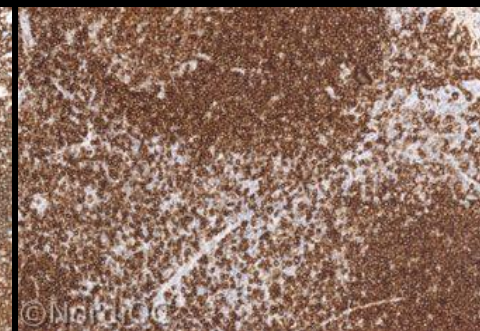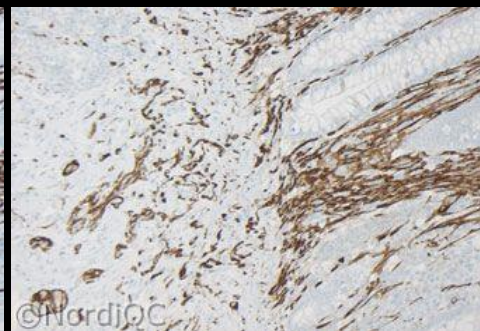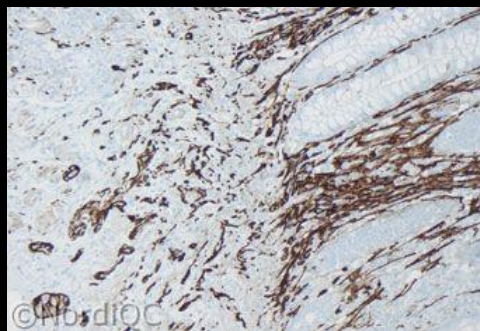

CD56

App – Tonsil – Neuroendocrine carc.

CD45


Tonsil – Liver – B-CLL.

Protocol A



Protocol B

Protocol A


Protocol B

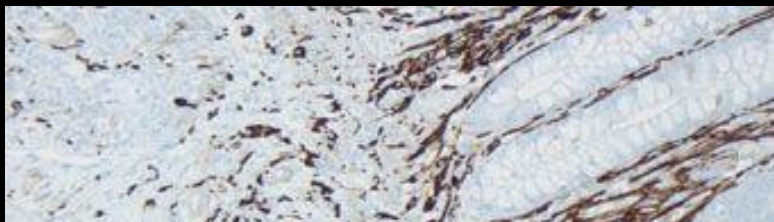

CD56: Optimal

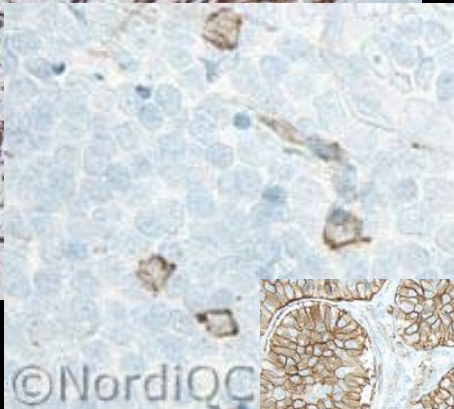

Insufficient....

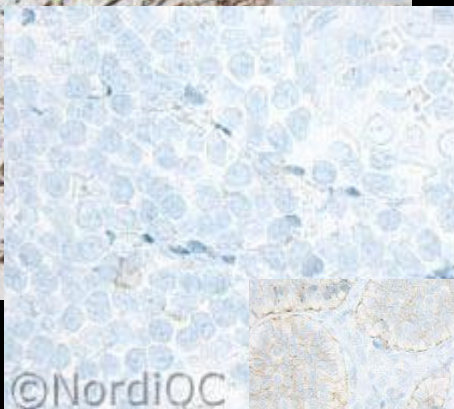

Tissues/cells with only high expression will not identify:

1. A poorly calibrated IHC assay
2. A reduced sensitivity in an optimally calibrated IHC assay

If an IHC test is used to demonstrate the target antigen being expressed at different levels, the controls must reflect this !

IHC Critical Assay Performance Controls (iCAPCs)

Which tissues are recommended ?

What is the expected staining pattern ?

Which tissues / cells are critical ?

Right antibody



Appropriate level of sensitivity

Guidance level of specificity

REVIEW ARTICLE

Standardization of Positive Controls in Diagnostic Immunohistochemistry: Recommendations From the International Ad Hoc Expert Committee

Emina E. Torlakovic, MD, PhD,† Søren Nielsen, HT, CT,‡§ Glenn Francis, MBBS, FRCPA, MBA, FFSc (RCPA),||¶## John Garratt, RT,†** Blake Gilks, MD, FRCPC,† †† Jeffrey D. Goldsmith, MD,‡‡ Jason L. Hornick, MD, PhD,*§§ Elizabeth Hyjek, MD, PhD,* Merdol Ibrahim, PhD,|| Keith Miller, FIBMS,|| Eugen Petcu, MD, PhD,|| Paul E. Swanson, MD,¶¶## Xiaoge Zhou, MD,**††† Clive R. Taylor, MD, PhD,‡‡‡ and Mogens Vyberg, MD,‡§*

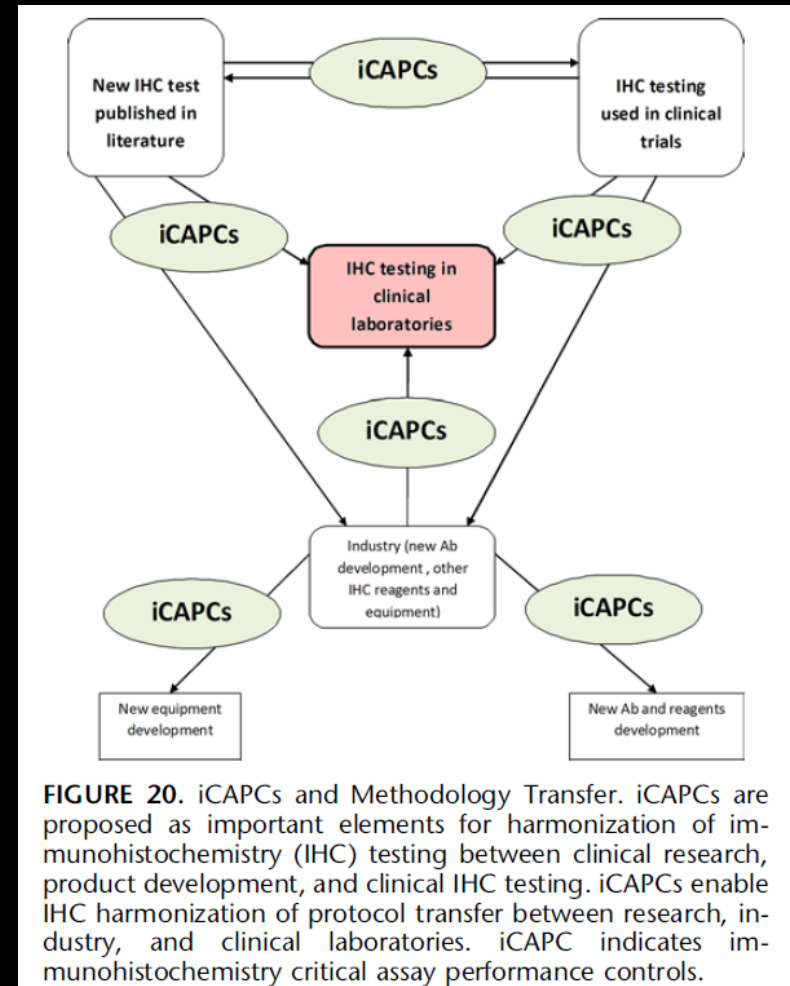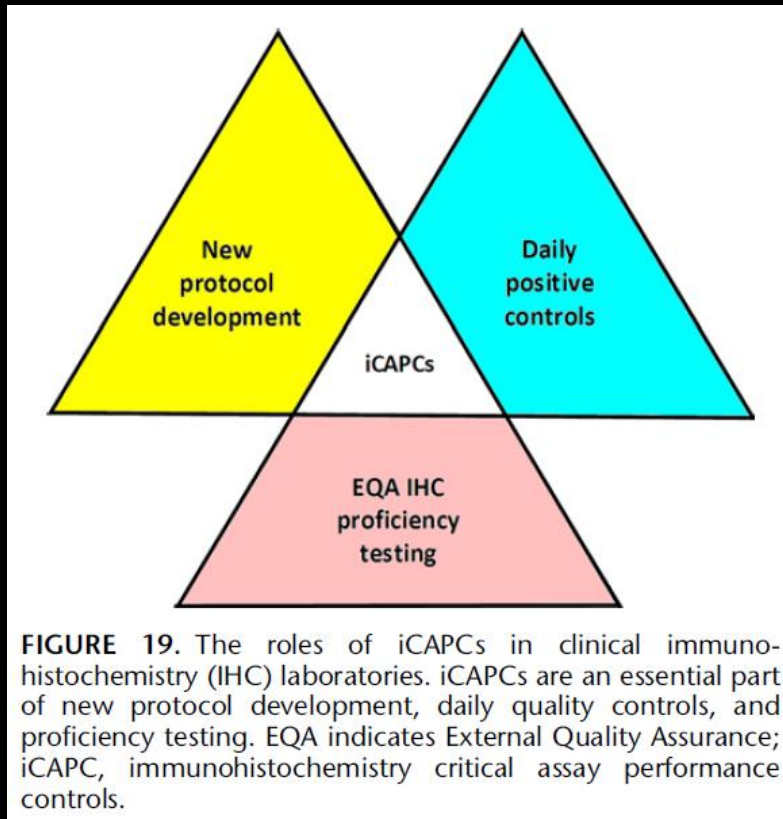

iCAPS to be used as central element for evaluation of quality;

Expected level – calibration

Analytical sensitivity and specificity

IHC – Biomarker controls

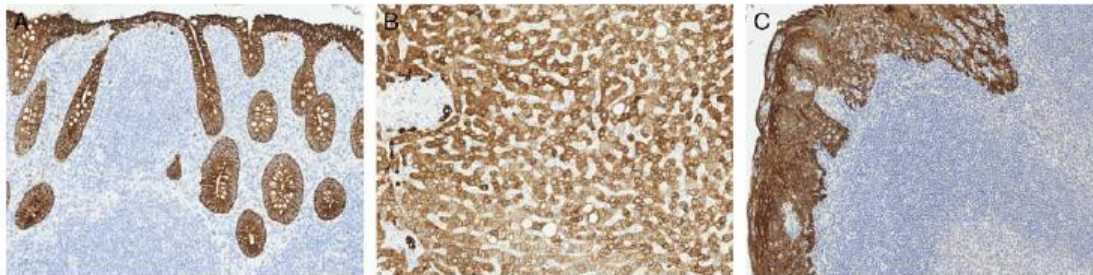


FIGURE 1. Pan-keratin iCAPC. A, Appendix: virtually all columnar epithelial cells must show a moderate to strong predominantly cytoplasmic staining reaction (a membranous accentuation will typically be seen). B, Liver: the vast majority of hepatocytes must show at least weak to moderate cytoplasmic staining reaction with a membranous accentuation (LLOD). C, Tonsil: all squamous epithelial cells must show a moderate to strong cytoplasmic staining reaction. Cytokeratin (CK)-positive interstitial reticulum cells (CIRCs) with dendritic/reticular pattern can show a weak to moderate cytoplasmic staining reaction (LLOD). iCAPC indicates immunohistochemistry critical assay performance controls; LLOD, low limit of detection.



FIGURE 7. TTF-1 iCAPC. A, Thyroid: virtually all epithelial cells must show a strong nuclear staining reaction. B, Lung: virtually all pneumocytes and basal cells of terminal bronchi must show a moderate to strong nuclear staining reaction. Columnar epithelial cells of terminal bronchi must show an at least weak nuclear staining reaction (LLOD). C, Tonsil: no staining reaction must be seen. iCAPC indicates immunohistochemistry critical assay performance controls; LLOD, low limit of detection.



FIGURE 8. CDX-2 iCAPC. A, Appendix: virtually all epithelial cells must show a strong nuclear staining reaction. A weak cytoplasmic staining reaction in addition to strong nuclear staining is often present. B, Pancreas: the majority of epithelial cells of intercalated ducts must show a weak to moderate nuclear staining reaction (LLOD). C, Tonsil: no staining reaction must be seen. iCAPC indicates immunohistochemistry critical assay performance controls; LLOD, low limit of detection.

Examples for 17 markers

General expected patterns

High expression
(Right antibody)

Low expression
(Appropriate sensitivity)

No expression
(Appropriate specificity)





Which tissue
Which cells
Which extension
Which intensity

IHC – Biomarker controls

	High express.	Low ex. (iCAPCs)	Non express.	Comment
CK-PAN	Appendix	Liver	Tonsil	
CK-LMW	Appendix	Liver	Tonsil	
CK-HMW	Tonsil	Pancreas	Liver	
CK7	Liver	Pancreas	Tonsil	
CK20	Appendix	Appendix	Tonsil	Different comp.
CD3	Tonsil	Appendix	Tonsil	
CD20	Tonsil	Appendix	Appendix	Different comp.
CD31	Tonsil	Liver	Appendix	
Vimentin	Appendix	Liver	Liver	Different comp.
Desmin	Appendix	Tonsil	Appendix	Different comp.
ASMA	Appendix	Liver	Appendix	Different comp.
SYP	Appendix	Appendix	Tonsil	Different comp.
CGA	Appendix	Appendix	Tonsil	Different comp.
TTF1	Thyroid	Lung	Tonsil	
CDX2	Appendix	Pancreas	Tonsil	
S100	Appendix	Tonsil	Appendix	Different comp.
Ki67	Tonsi ¹	Tonsil	Tonsil	Different comp.

IHC – Biomarker controls

ASMA (C)	Appendix	Liver	Pancreas	Tonsil
High expression (right ab)	A moderate to strong staining reaction in virtually all smooth muscle cells in muscularis mucosae	A moderate to strong staining reaction in the smooth muscle cells in vessels	A moderate to strong staining reaction in the smooth muscle cells in vessels	A moderate to strong staining reaction in the smooth muscle cells in vessels
Low expression iCAPCs (right sens.)	-	An at <u>least weak to moderate</u> , staining reaction of the <u>majority of the perisinusoidal cells</u>	-	-
Non expression (right spec.)	No staining reaction in the epithelial cells	No staining in the hepatocytes (except lipofuscin)	No staining reaction in the epithelial cells	No staining reaction in lymphocytes

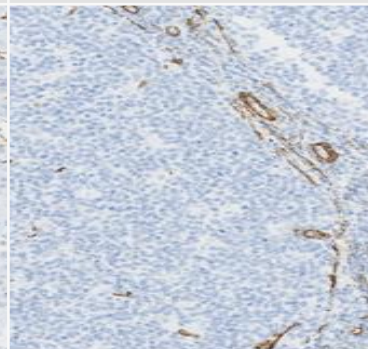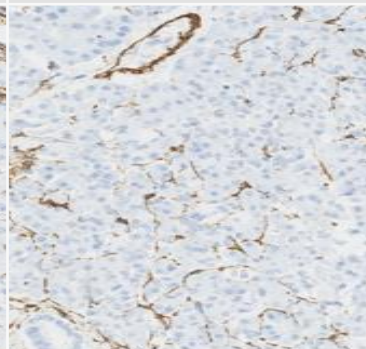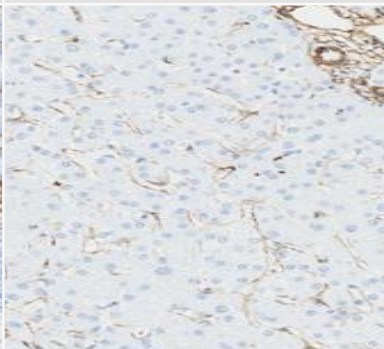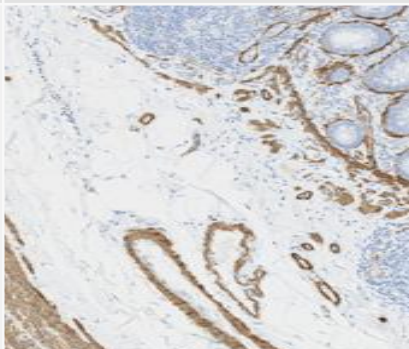

- The NordiQC focus areas
 - Central protocol elements for an optimal staining
 - Antibody selected
 - Antibody dilution range / Ready-To-Use
 - Epitope retrieval
 - IHC detection system & stainer platforms
 - Recommendable control and identification of critical quality stain indicators / iCAPCs
(Which tissue ? Which cells ?, How must they look ?)

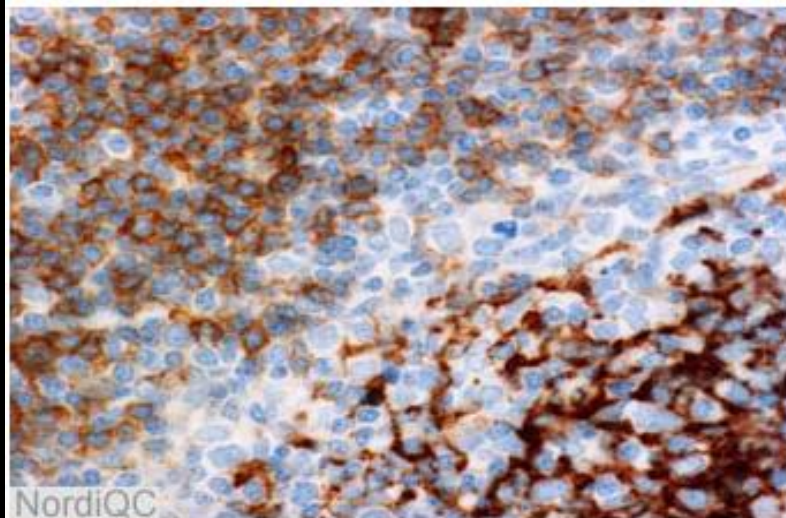


Fig. 2a. High magnification of the optimal staining in Fig 1a of the secondary follicle in the tonsil. The activated B-cells show a distinct continuous membranous reaction.

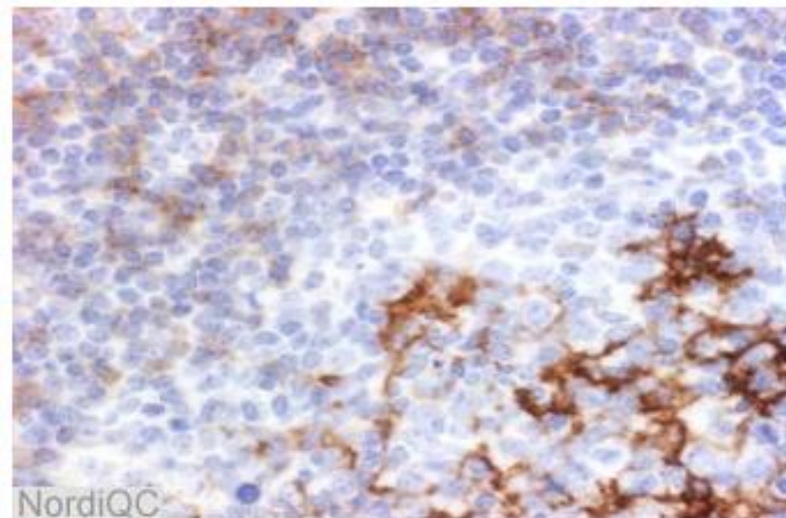


Fig. 2b. High magnification of the insufficient staining in Fig 1b of the secondary follicle in the tonsil (same field as in Fig 2a). The activated B-cells only show a weak imprecise reaction.

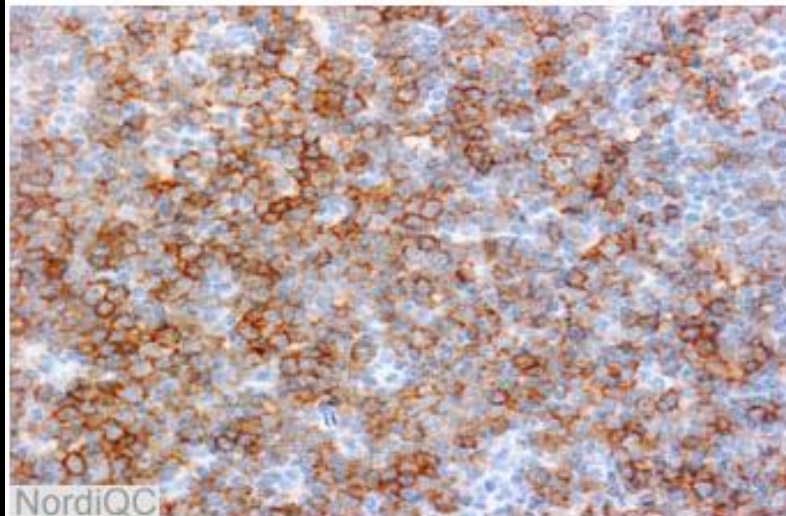


Fig. 3a. Optimal staining for CD23 of the B-CLL no 4 using same protocol as in Fig 1b and 2 b. The majority of the neoplastic cells show a strong and distinct membranous staining.

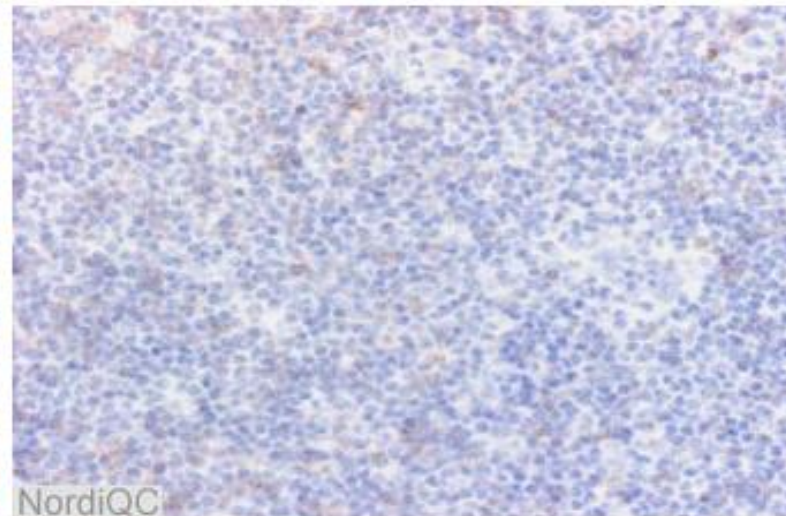


Fig. 3b. Insufficient staining for CD23 of the B-CLL no 4 using same protocol as in Fig 1b and 2 b. The neoplastic cells are virtually negative.

CD23

iCAPCs:

Activated
B-cells in
mantle z.

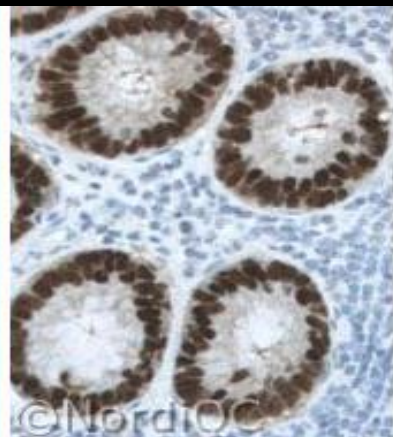


Fig. 1a. Optimal staining for CDX2 using the mAb clone CDX2-88.
Left, colon: A strong nuclear staining is seen in all the enterocytes with a minimal cytoplasmic reaction.
Right, pancreas: A weak to moderate staining is seen in the majority of the ductal epithelial cells.

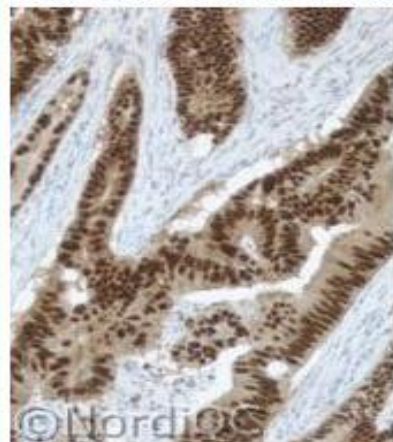


Fig. 2a. Optimal staining for CDX2 using same protocol as in Fig. 1a.
Left: Colon adenocarcinoma with high expression of CDX2: The nuclei of the neoplastic cells show an intense staining while the cytoplasmic compartment is weakly stained.
Right: Colon adenocarcinoma with low expression of CDX2: The majority of the neoplastic cells show a moderate to strong nuclear reaction.

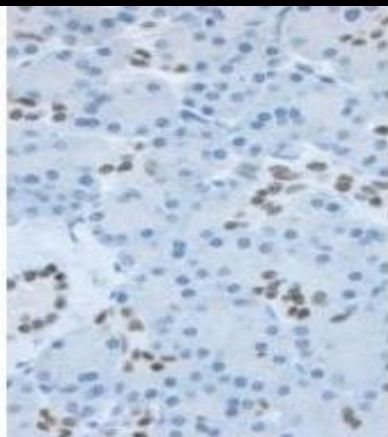


Fig. 1b. Staining for CDX2 using the mAb clone CDX2-88 with an insufficient protocol.
Left, colon: A moderate to strong nuclear staining is seen in all the enterocytes.
Right, pancreas: No nuclear staining is seen in the ductal epithelial cells. Also compare with Fig 2b – same protocol.

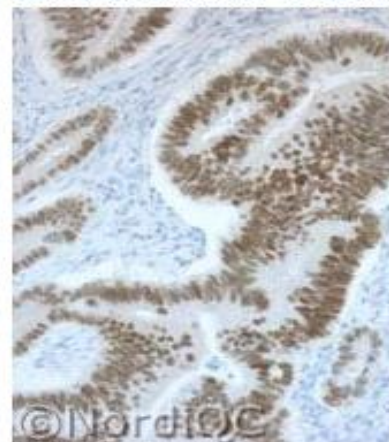


Fig. 2b. Insufficient staining for CDX-2 using same protocol as in Fig. 1b.
Left: Colon adenocarcinoma with high expression of CDX2: The nuclei of the neoplastic cells show a moderate staining, while the cytoplasmic compartment is almost negative.
Right: Colon adenocarcinoma with low expression of CDX2: Only scattered neoplastic cells show a weak nuclear reaction.

CDX2

iCAPCs:

Pancreatic
duct ep.
cells

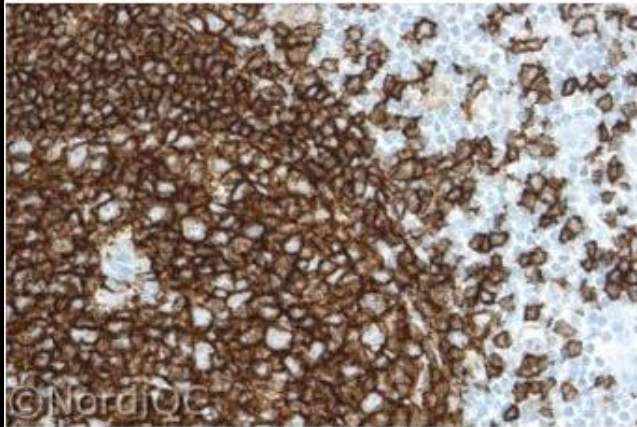


Fig. 1a. Lymphatic tissue in the appendix showing an optimal staining reaction for CD20 using the mAb clone L26 in a RTU format on the BenchMark platform. HIER was performed using Cell Conditioning 1. A very strong membranous staining reaction is seen in virtually all the B-cells.

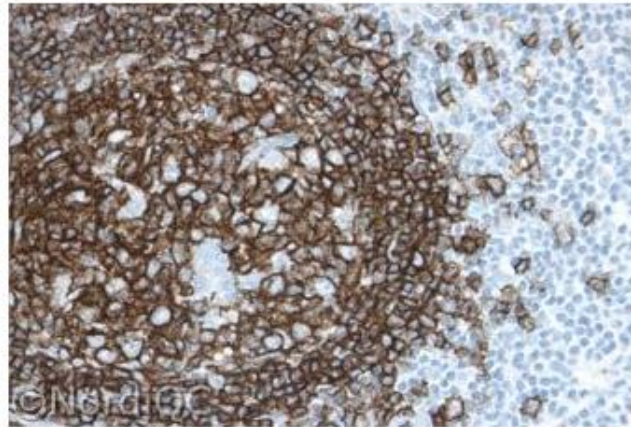


Fig. 1b. Lymphatic tissue in the appendix. Same field as in Fig. 1a. Insufficient staining for CD20 using the mAb clone L26 in a RTU format at the BenchMark platform. No HIER was performed. A moderate to strong staining reaction is seen in virtually all the B-cells. The normal B-cells are high expressors of CD20, hence the relatively strong reaction. Even so, the staining intensity should be improved in order to detect low expressors of CD20 (e.g. B-CLL in Fig. 2a and 2b).

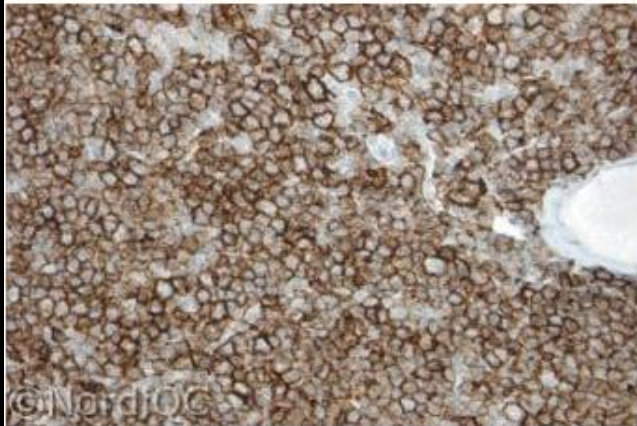


Fig. 2a. B-CLL. Optimal staining reaction for CD20. Same protocol as in Fig. 1a. A moderate to strong membranous staining is seen in virtually all the neoplastic cells.

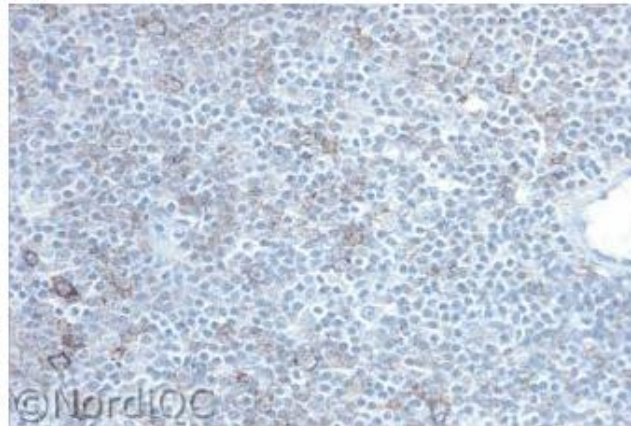


Fig. 2b. B-CLL. Insufficient staining for CD20 using the same protocol as in Fig. 1b. Omitting HIER, only scattered cells are positive. The majority of the neoplastic cells are negative. Compare with the optimal result in Fig. 2a, same field.

CD20:

iCAPCs:

????

ASAP....

As strong as possible...

IHC – Biomarker controls

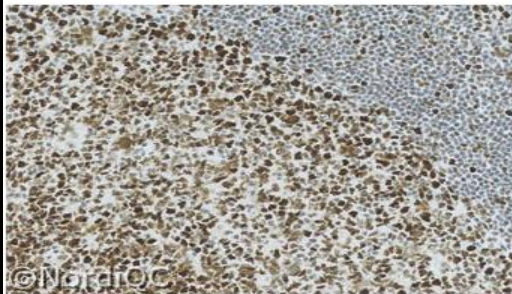


Fig. 1a. Optimal staining for MSH6 of the tonsil using the mAb clone EP49 optimally calibrated, HIER in an alkaline buffer and a 3-step polymer based detection system. Virtually all the mantle zone B-cells show a distinct, moderate to strong nuclear staining, while the germinal centre B-cells show a strong nuclear staining.

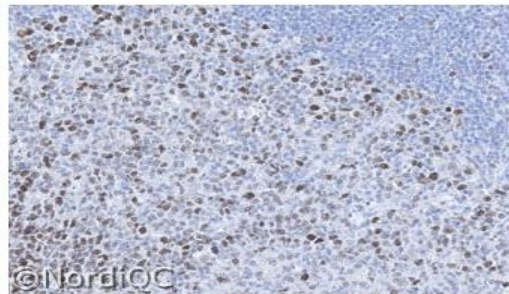


Fig. 1b. Insufficient staining for MSH6 of the tonsil using the mAb clone 44. by a protocol with a too low sensitivity (2-step polymer and too low. conc. of the primary Ab), same field as in Fig. 1a. Only the germinal centre B-cells are demonstrated, while the mantle zone B-cells expressing limited MSH6 are virtually unstained. Also compare with Figs. 2b. & 3b., same protocol.

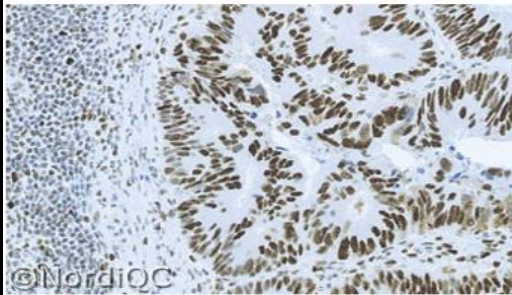


Fig. 2a. Optimal staining for MSH6 of the colon adenocarcinoma no. 3 with intact MSH6 protein using same protocol as in Fig. 1a. The majority of the epithelial and the stromal cells show a moderate to strong nuclear staining. No background staining is seen.

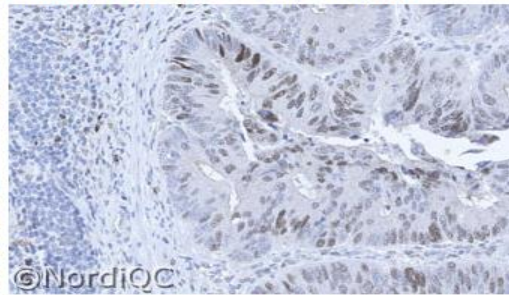


Fig. 2b. Insufficient staining for MSH6 of the colon adenocarcinoma no. 3 with intact MSH6 protein using same protocol as in Fig. 1b., same field as in Fig. 2a. The proportion of positive cells and the intensity of the staining reaction is significantly reduced compared to the result in Fig. 2a. Also compare with Fig. 3b., same protocol.

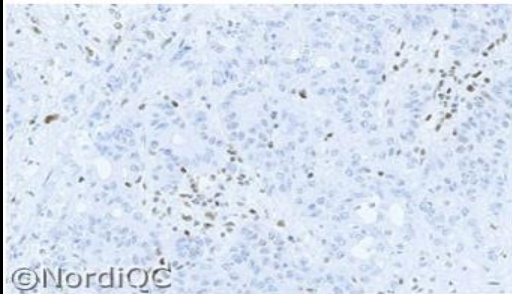


Fig. 3a. Optimal staining for MSH6 of the colon adenocarcinoma no. 5 with loss of MSH6 protein using same protocol as in Figs. 1a. & 2a. The neoplastic cells are negative, while the remnants of entrapped lymphocytes and stromal cells show a distinct nuclear staining, serving as internal positive control.

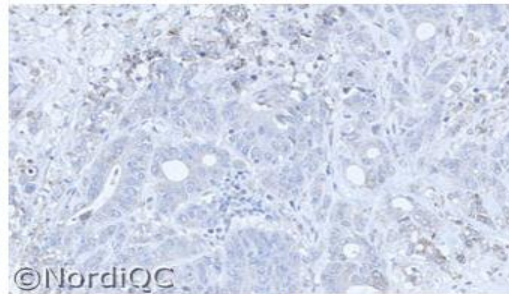


Fig. 3b. Insufficient staining for MSH6 of the colon adenocarcinoma no. 5 with loss of MSH6 protein using same protocol as in Figs. 1b. & 2b., same field as in Fig. 3a. No nuclear staining reaction is seen in the neoplastic cells, but as virtually no nuclear staining reaction is seen in the normal cells as stromal cells, the staining pattern can not reliably be interpreted. Also note the weak cytoplasmic staining complicating the interpretation.

MMR:


iCAPCs:

Mantle zone B-cells
in tonsil

+++++++

(internal control)





Stromal cells!!

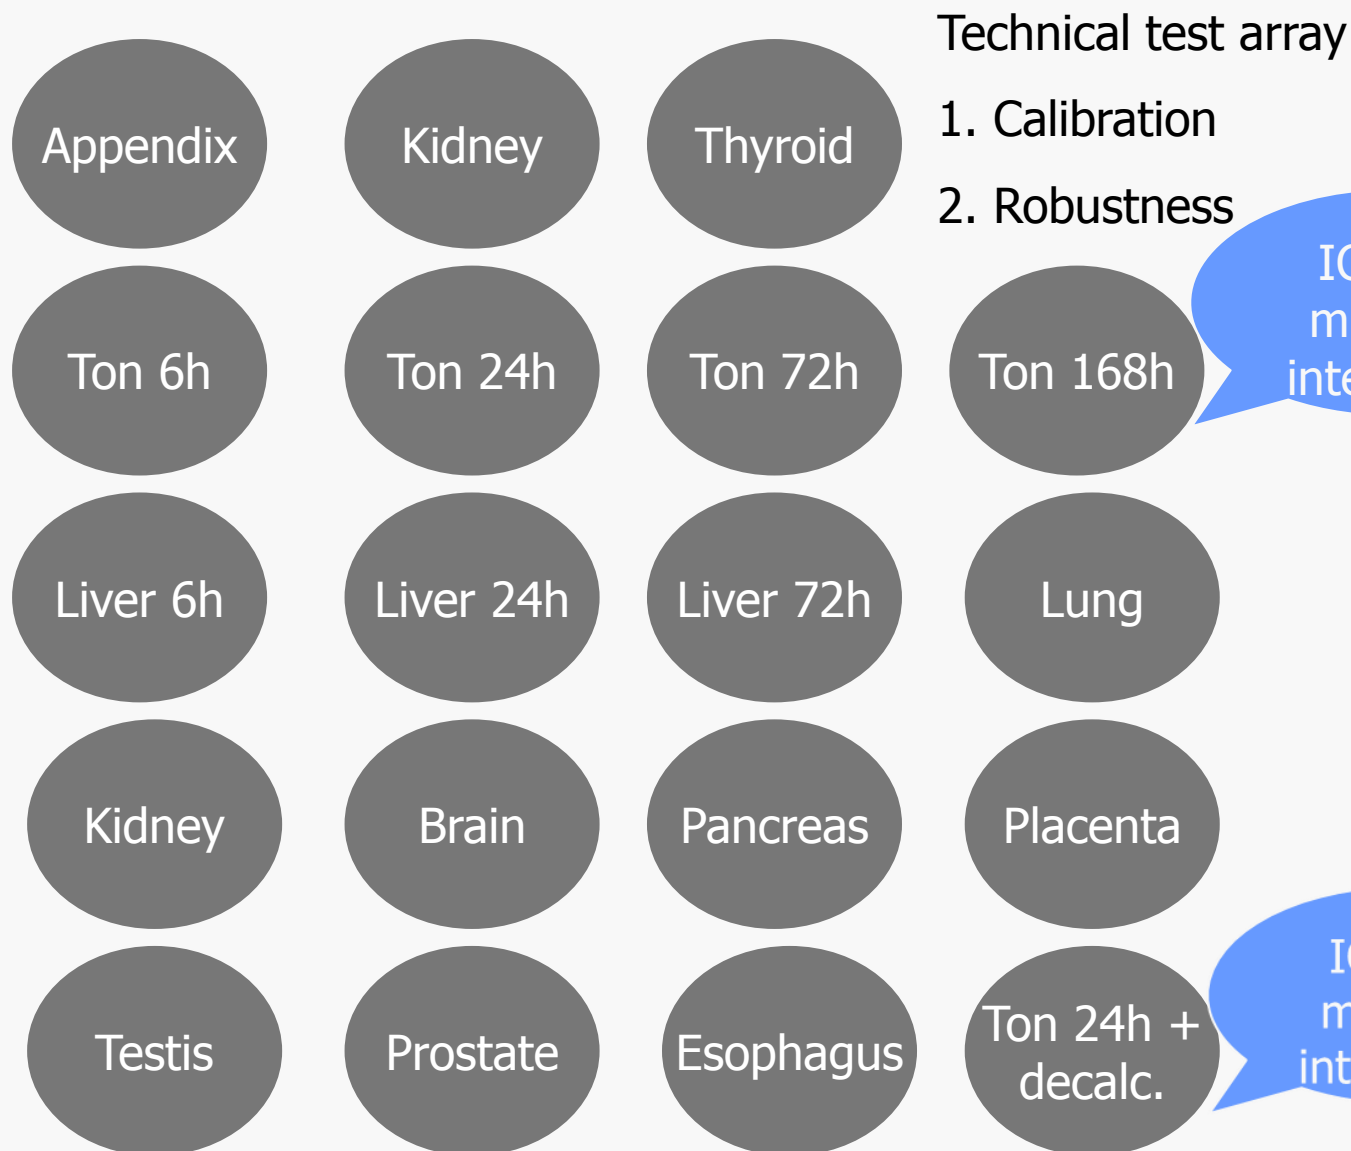

Protocol set-up: used as primary material for the calibration of 130 of 195 routine diagnostic markers, Aalborg University Hospital

IHC – Biomarker controls

Colon: S100, polyclonal

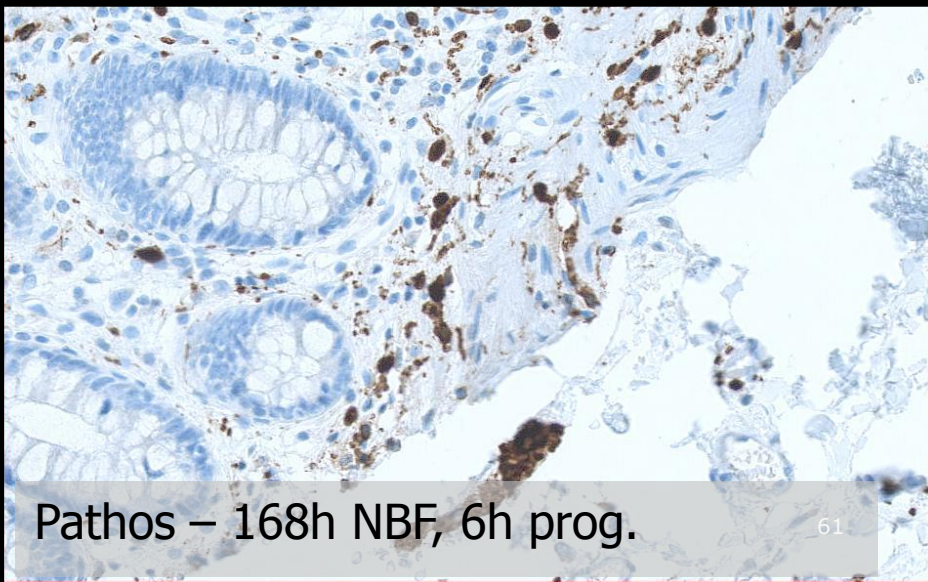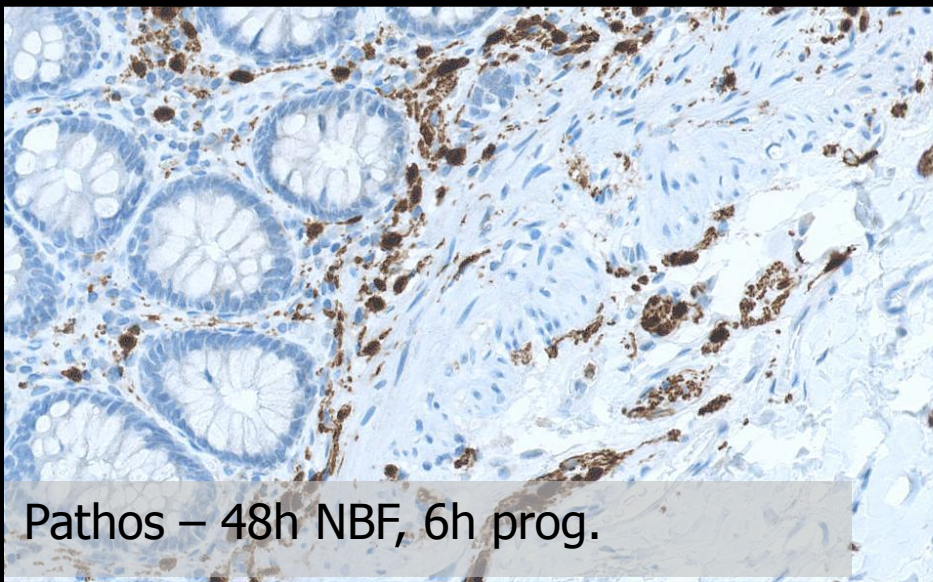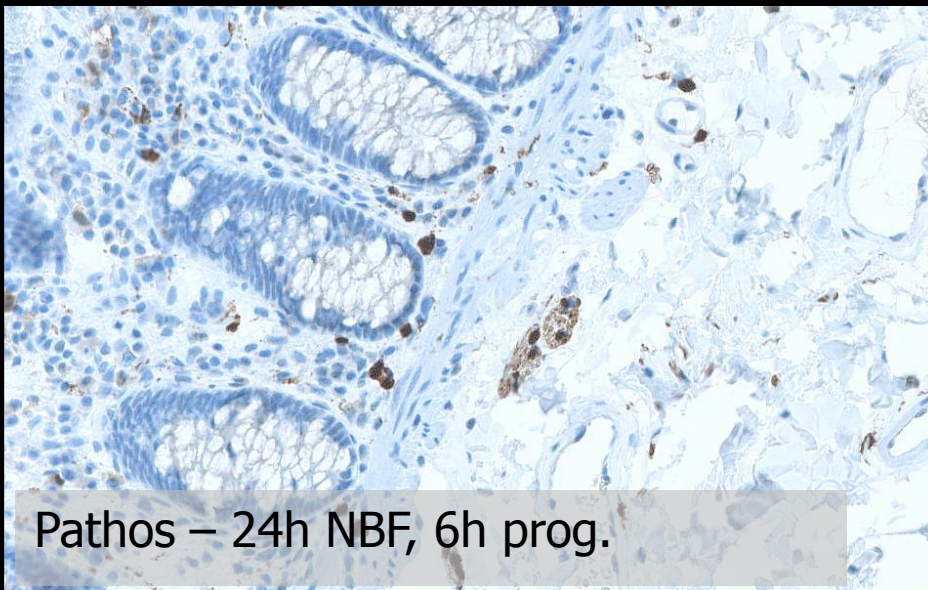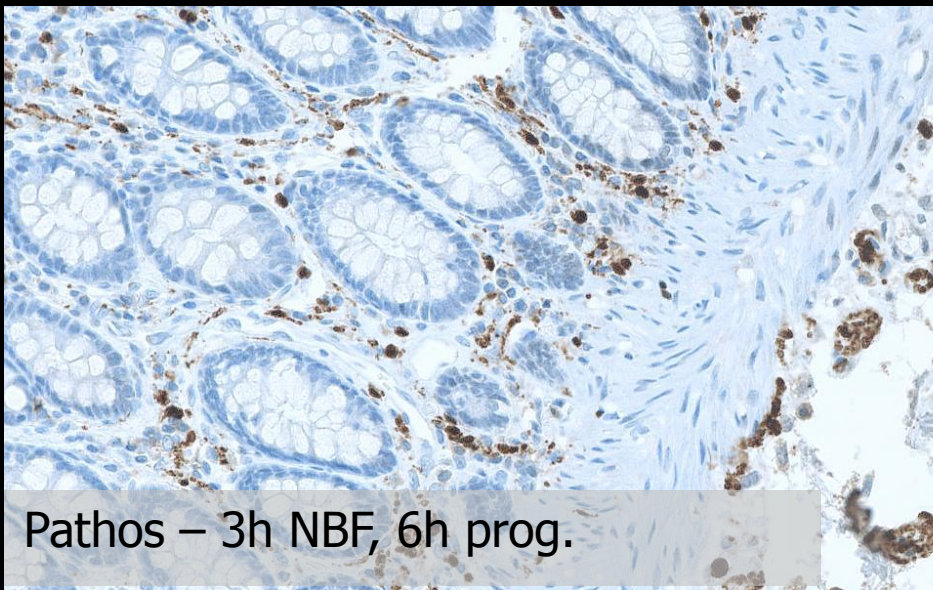

IHC – Biomarker controls

Tonsil: S100, polyclonal

S100 = Soluble in 100% alcohol

Pathos – 3h NBF, 2h prog.

Pathos – 24h NBF, 2h prog.

Pathos – 48h NBF, 2h prog.

Pathos – 168h NBF, 2h prog.


Concentrated antibodies – Aalborg Hospital (app. 200 Abs) – VMS ULTRA

	1:25	1:100	1:400
A	None	None	None
B	Enzyme P1, 4 min	Enzyme P1, 4 min	Enzyme P1, 4 min
C	HIER CC1 pH 8.5*	HIER CC1 pH 8.5	HIER CC1 pH 8.5
D	HIER CC2 pH 6.0*	HIER CC2 pH 6.0	HIER CC2 pH 6.0

(E)	CC1 + Enzyme P3, 8 min	CC1 + Enzyme P3, 8 min	CC1 + Enzyme P3, 8 min
(F)	Enzyme P3, 8 min + CC1	Enzyme P3, 8 min + CC1	Enzyme P3, 8 min + CC1

*HIER time 48 min. at 99°C
OptiView DAB

1. Technical calibration

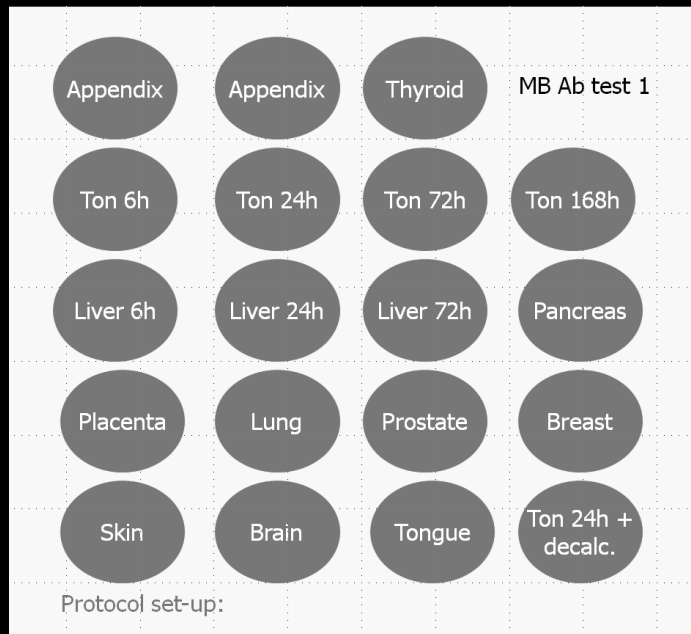

2. Diagnostic / analytical evaluation

- Analytical validation

- Laboratory developed tests (concentrates and RTU formats being applied modified to official protocol)

- Non-predictive markers (- ER, PR, HER-2..)

- CLSI: 20 cases per entity relevant (pos, neg)

- CAP: 10 positive, 10 negative



- The validation set should include high and low expressors for positive cases when appropriate and should span the expected range of clinical results (expression levels) for markers that are reported quantitatively.

- Ad-Hoc: 10 strongly pos, 10 interm. to low, 5 neg.



Number less important compared to use of tissue with full range of expression patterns reflecting the diagnostic use

IHC – Biomarker controls



Lung squam. cell carc.

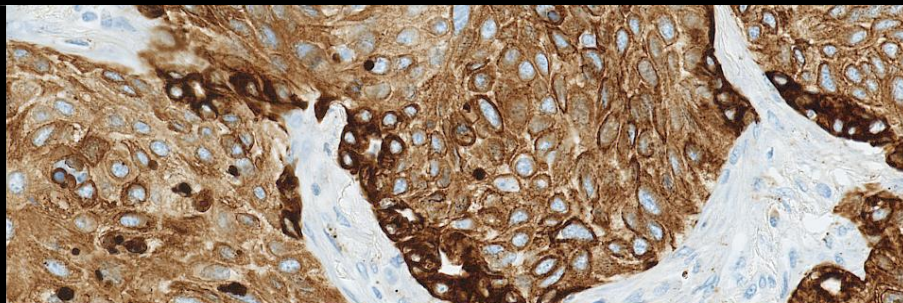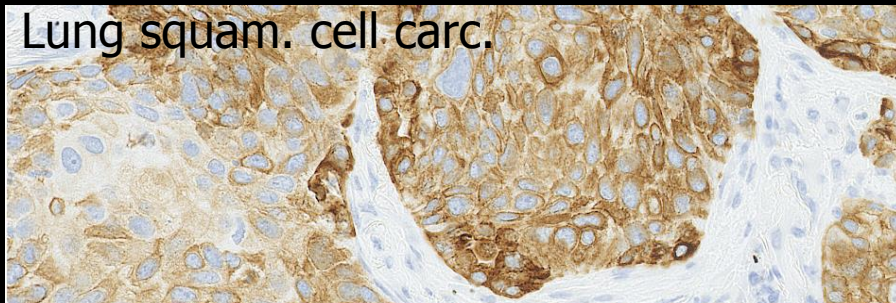



Lung ad. carc.

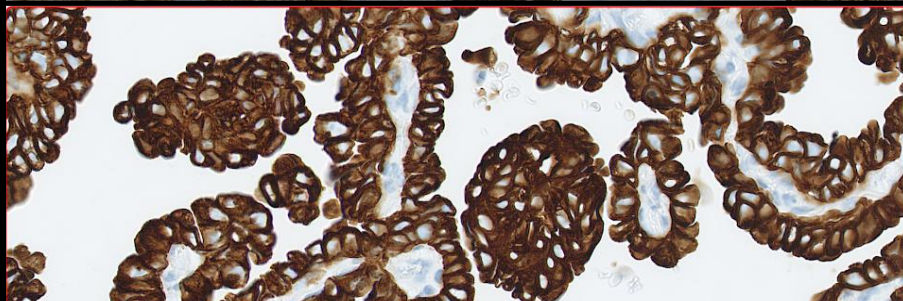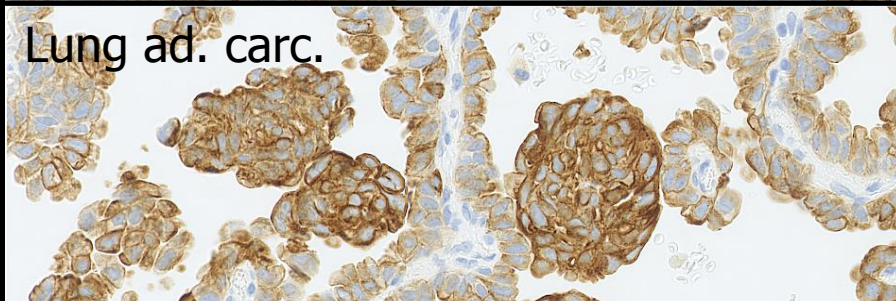

SCLC

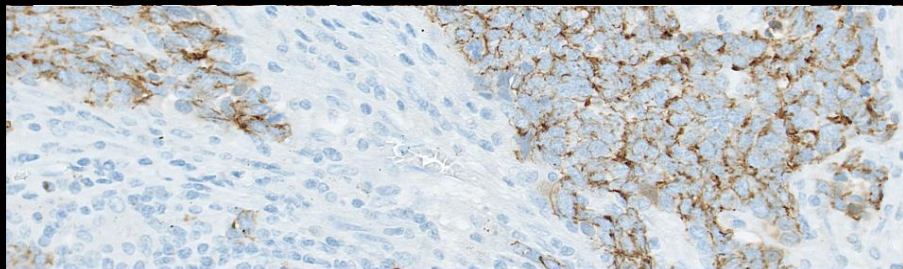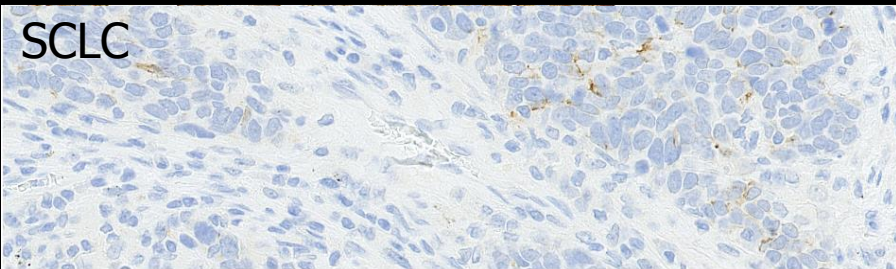


RCC

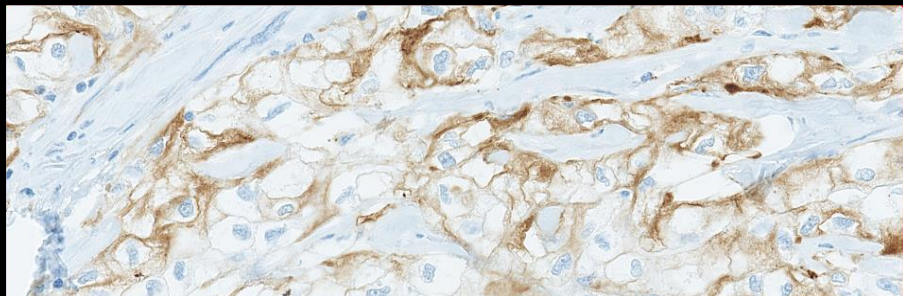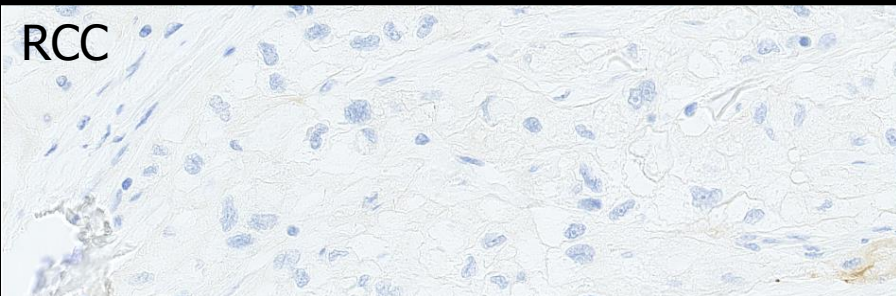

CK-PAN - mAb AE1/AE3 – Prot. 1

CK-PAN - mAb AE1/AE3 – Prot. 2

IHC – Biomarker controls

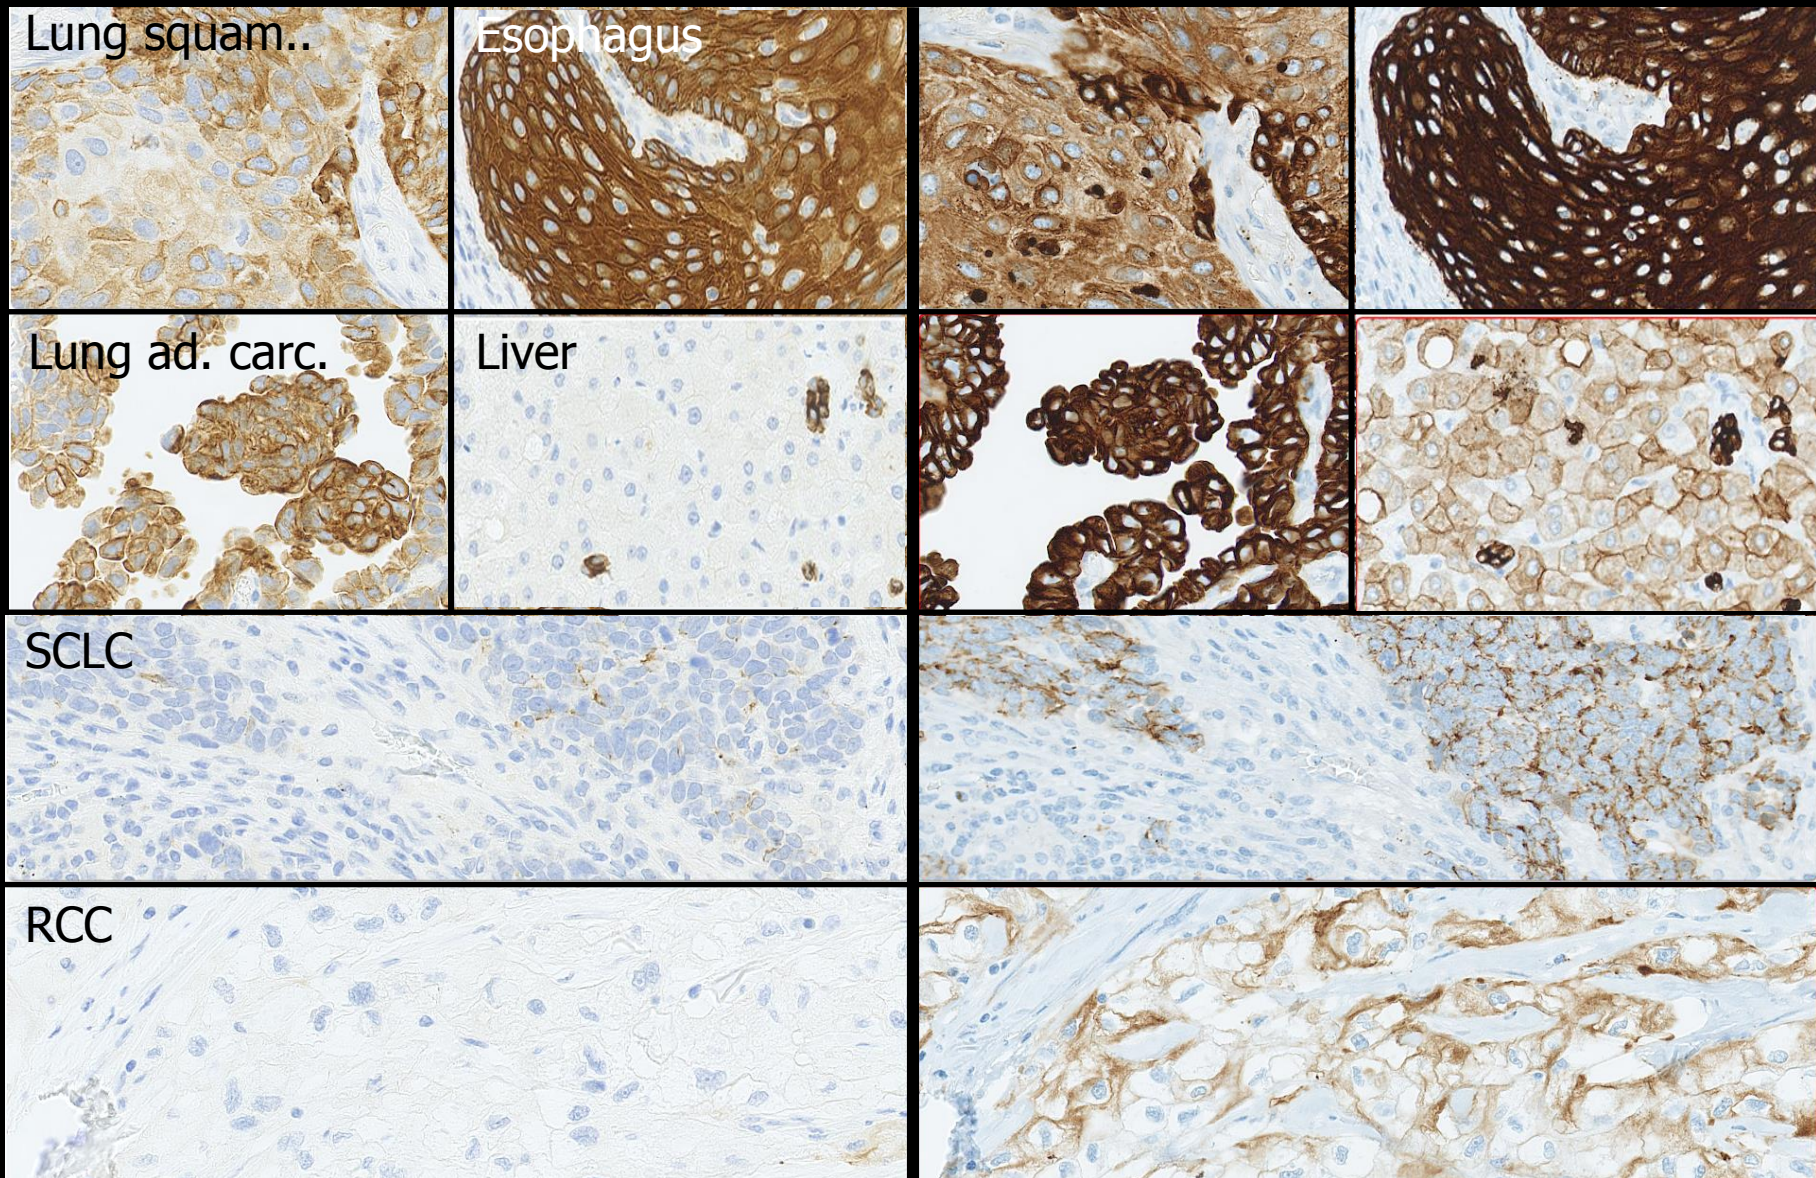

CK-PAN - mAb AE1/AE3 – Prot. 1

CK-PAN - mAb AE1/AE3 – Prot. 2

IHC – Biomarker controls

Analytical Index / sensitivity TMA

Tumor 1

Tumor 2

Tumor 5

Tumor 6

Tumor 9

Tumor 10

Tumor 12

Tumor 13

Diagnostic potential:

Index and accuracy TMA's

TMA Neoplasia

Analytical accuracy / specificity TMA

Liver

Mamma
ductal
carc.

Mamma
ductal
carc.

Mamma
Lobular
carc.

Lung
adeno
carc.

Lung
adeno
carc.

Lung
squam.
carc.

Colon
adeno
carc.

Colon
adeno
carc.

Kidney
clear c
carc.

Kidney
clear c
carc.

Thyroid.
follic.
carc.

Thyroid.
Medul.
carc.

Ovary.
Serous I
carc.

Ovary.
Serous I
carc.

Ovary.
Clear
carc.

Ovary.
Endom.
carc.

Corpus
Uteri
Endom.
carc.

Cervix
Uteri
adeno
carc.

Tonsil

Testis
Semin.

Testis
Semin.

Prostate
adeno
carc.

Prostate
adeno
carc.

Intest
Carcinoid

Melanom

Melanom

Pancr.
adeno
carc.

Pancr.
adeno
carc.

Uroth.
carc.

Uroth.
carc.

GIST

Leio
myo
sarcoma

Rhabdo
myo
sarcoma

Hodgkin
Classic

Hodgkin
mixed

Diffuse
large B
lymph.

Diffuse
large B
lymph.

B-CLL

Follik.
lymph


Mantle
cell
lymph.

T-cell
lymph.
perip.


T-cell
lymph.
Anapl.

IHC – Biomarker controls


CD117 TMA: 16 x GIST

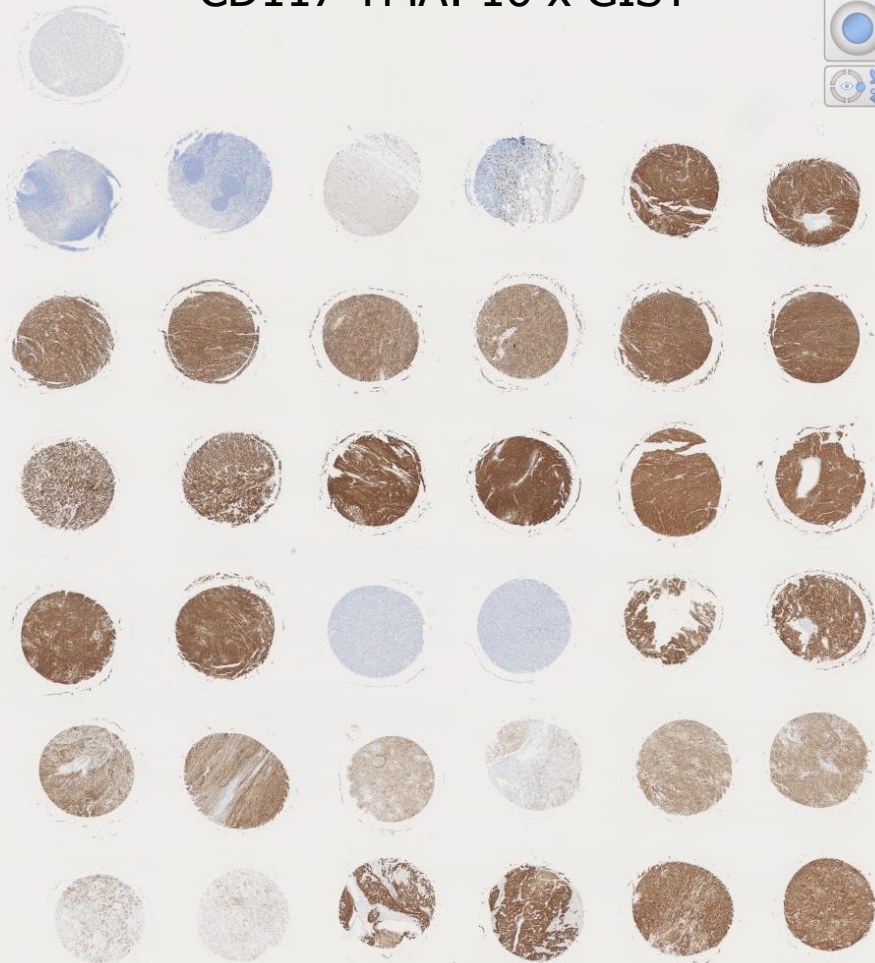



Neoplasias TMA: 42 x

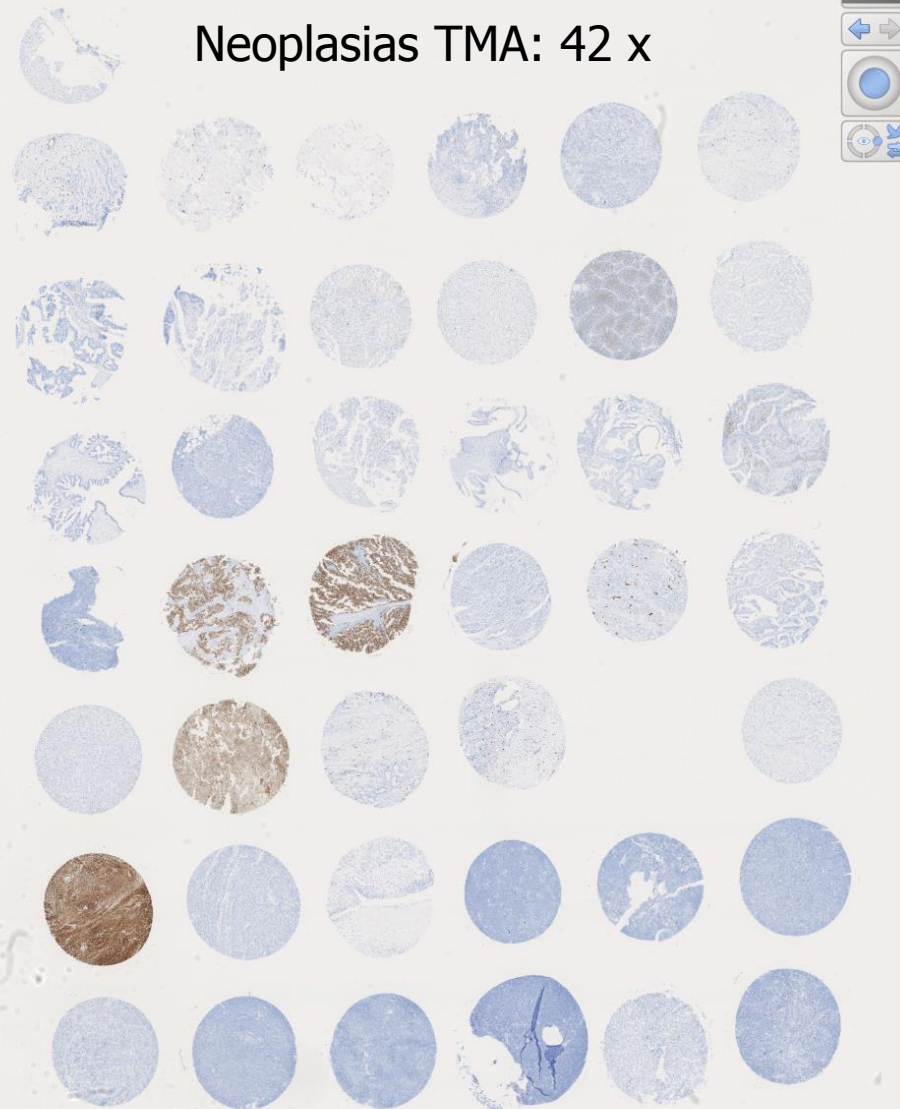


IHC – Biomarker controls

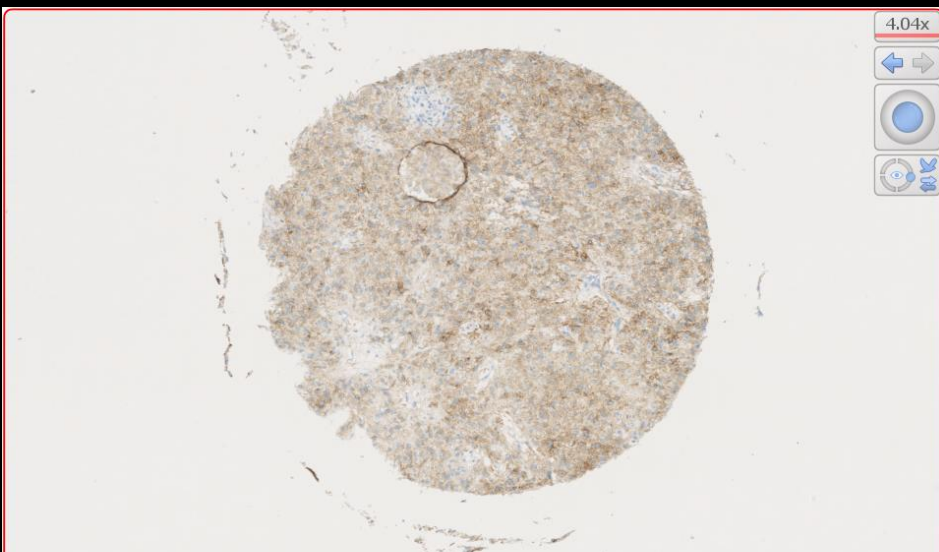

CD117 TMA: 16 x GIST

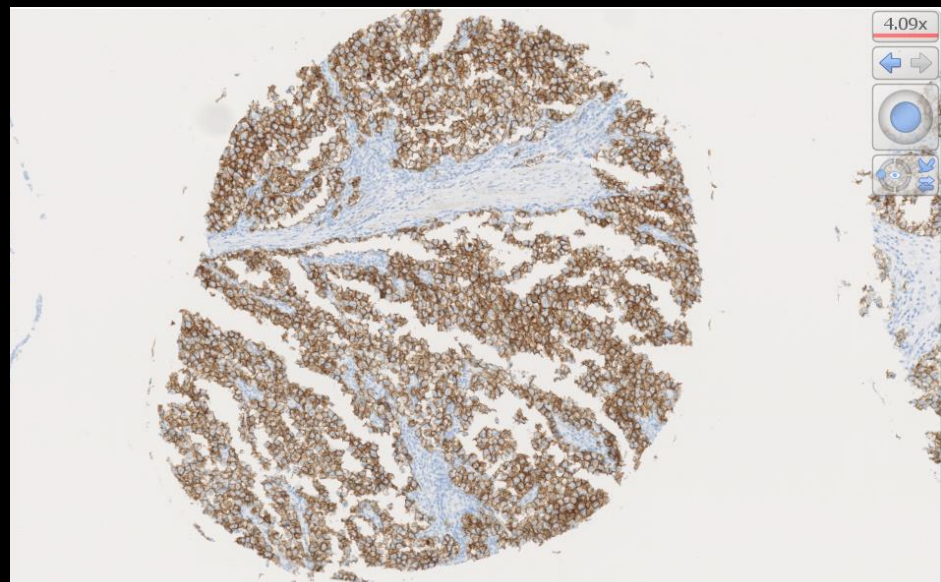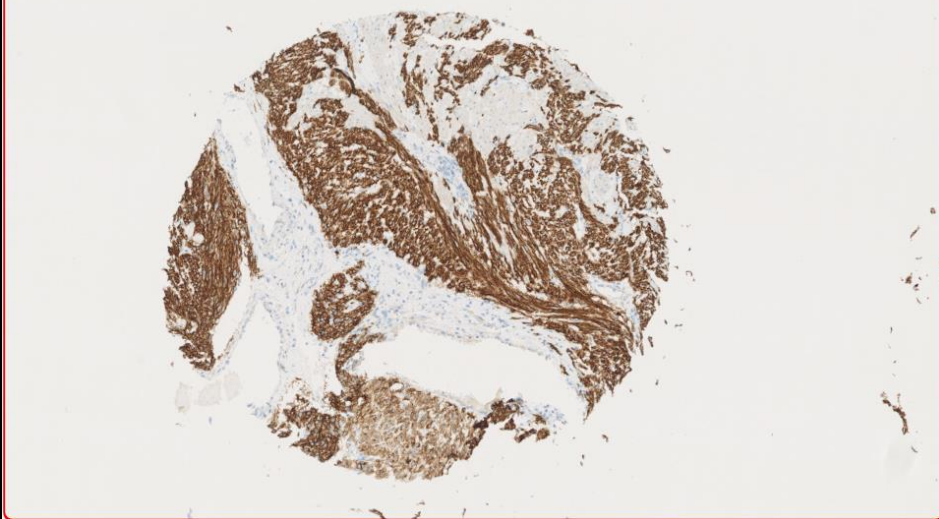


Neoplasias TMA: 42 x

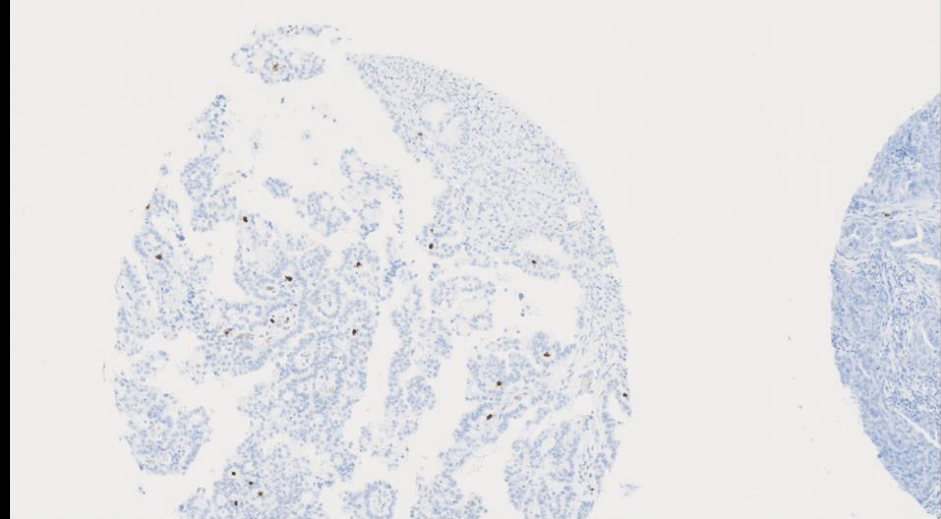

NordiQC – Antibodies giving different patterns

Antigen	Clone	High expressor	Low expressor	Non expressor
CD3	LN10, 2GV6	✓	✓	—
CD3	Poly A0452	✓	✓	(+) — (epith.)
CD5	SP19	✓	✓	—
CD5	4C7	✓	✓	(+) — (epith.)
CD8	4B11,C8/144B	✓	✓	—
CD8	SP57	✓	✓	(+) — (epith.)
MUM1	EUA32, MUM1p,	✓	✓	—
MUM1	MRQ-43	✓	✓	(+) — (epith.)
OCT 3/4	C10, N1NK	✓	✓	—
OCT 3/4	MRQ-10	✓	✓	+ — (neuroendo.)
PLAP	NB10	✓	✓	—
PLAP	8A9	✓	✓	+ — (muscle)
WT1	WT49	✓	✓	—
WT1	6F-H2	✓	✓	+ — (epith.)


IHC – Biomarker controls

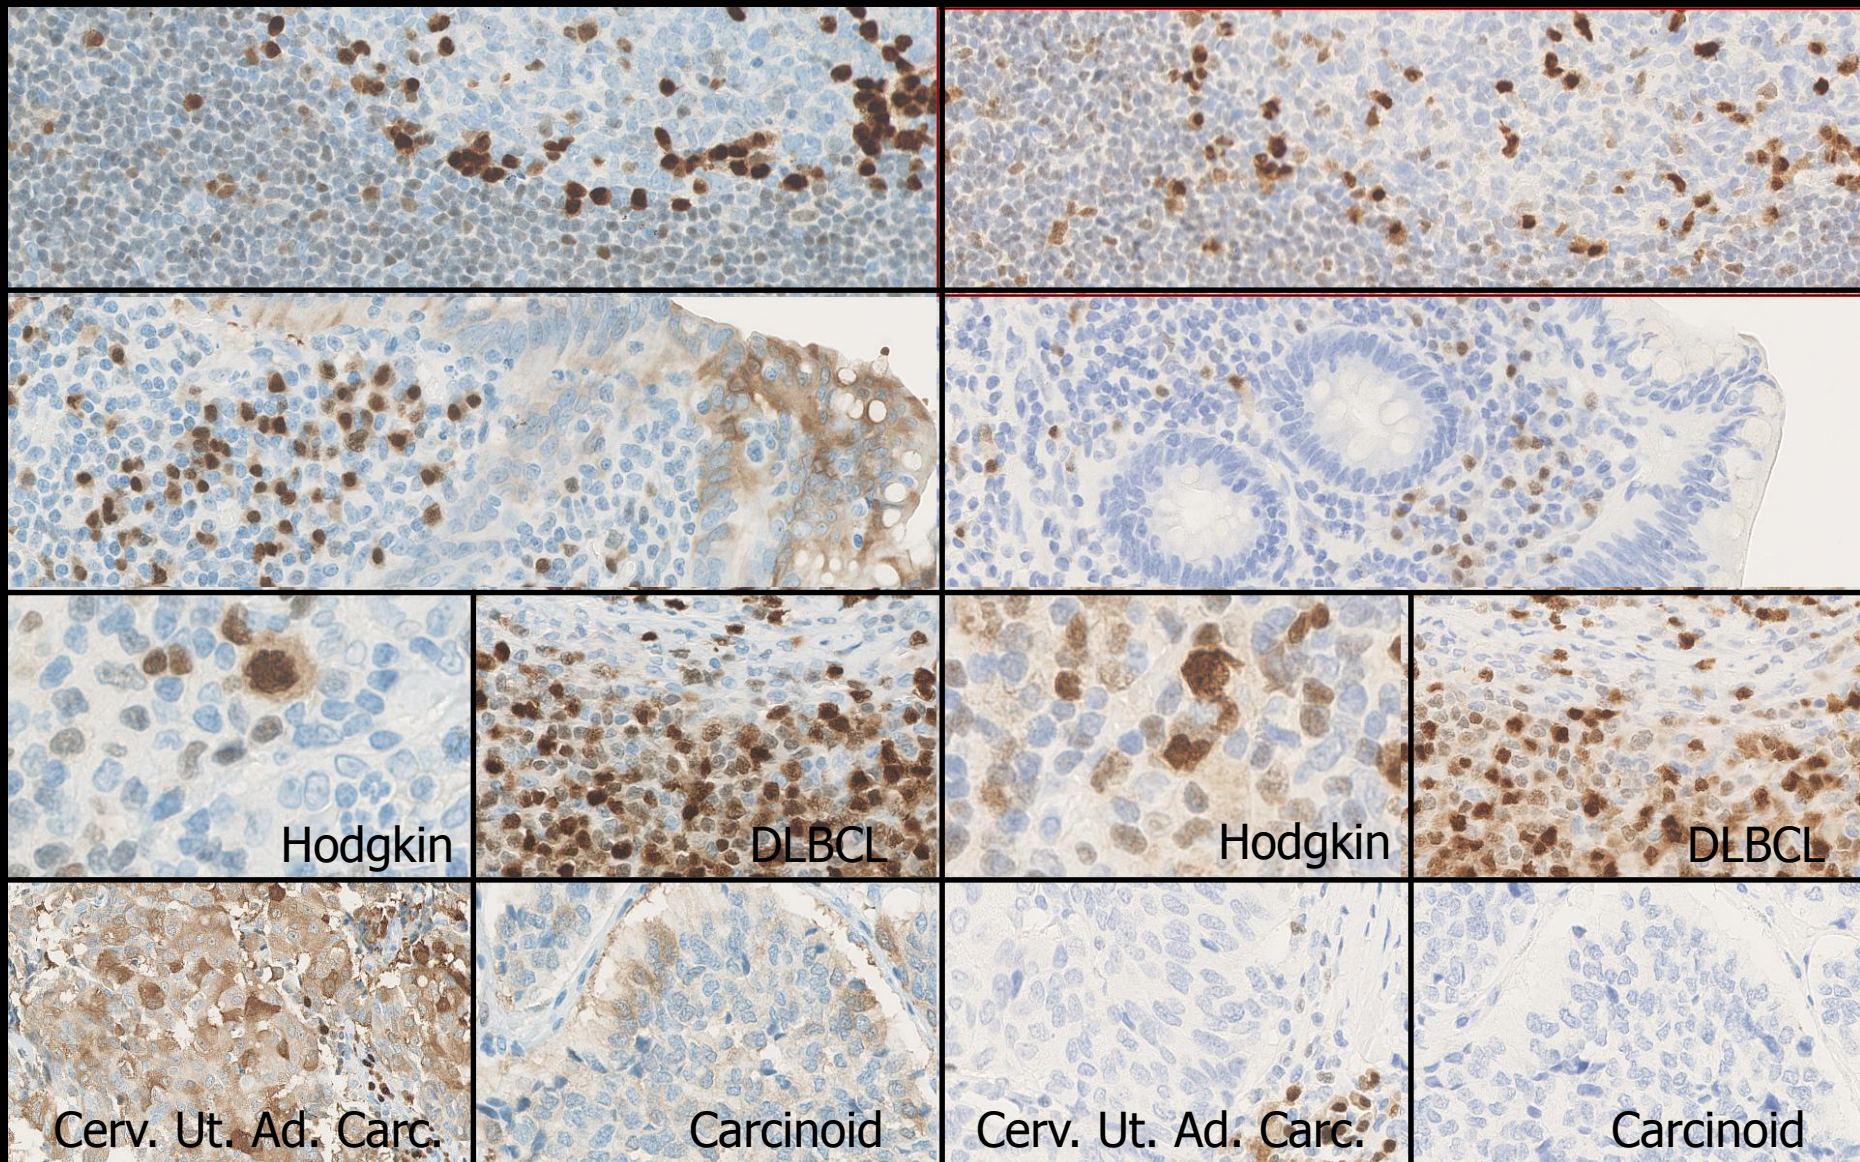

MUM1 - mAb MRQ-43

MUM1 - mAb EUA32 & MUM1p






IHC – Biomarker controls

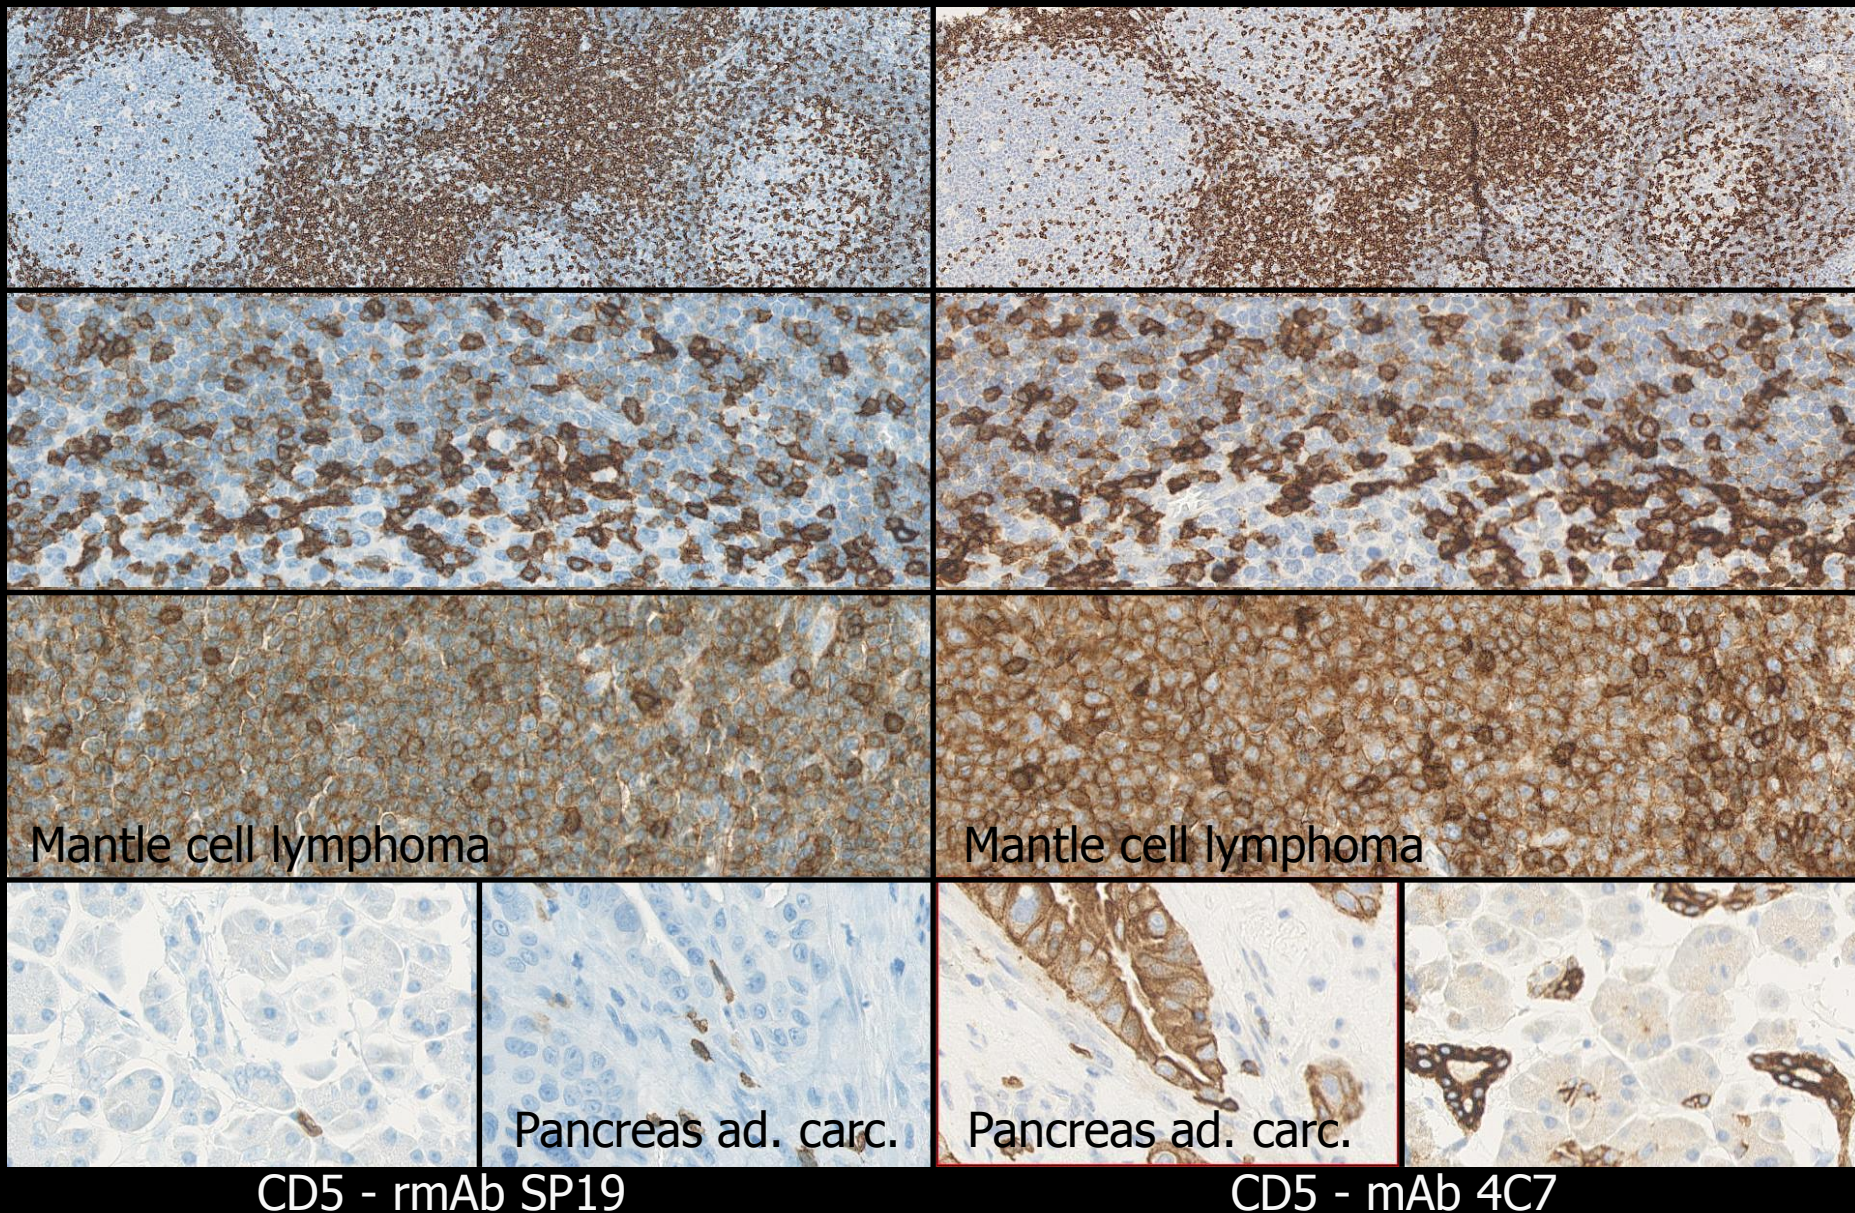

NordiQC – Less successful antibodies

Antigen	Clone	High expressor	Low expressor	Non expressor
CD5	CD5/54/F6	√	FN	—
CD23	MHM6	√	FN	—
CD31	1A10	(√)	FN	—
CD31	SP38	(√)	FN	—
CD138	5F7	(√)	FN	—
CDX2	SP54	(√)	FN	FP
CEA	TF-3H8-1	√	√	FP
CGA	DAK. A3	√	FN	—
CK20	PW31	√	(√)	—
CK-LMW	35BH11	√	FN	—
MLH1	EPR3894	√	√	FP
MSH2	EPR3943	√	√	FP
MSH6	44	√	FN	XB
SYP	SY38	√	FN	XB 73

IHC – Biomarker controls

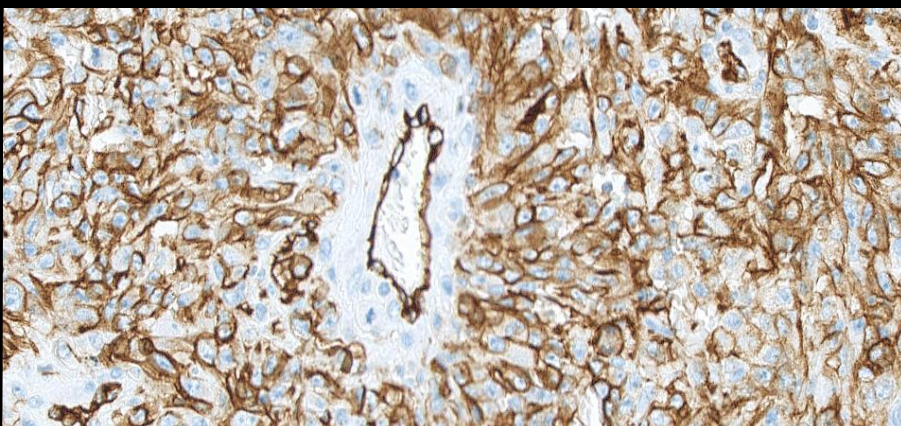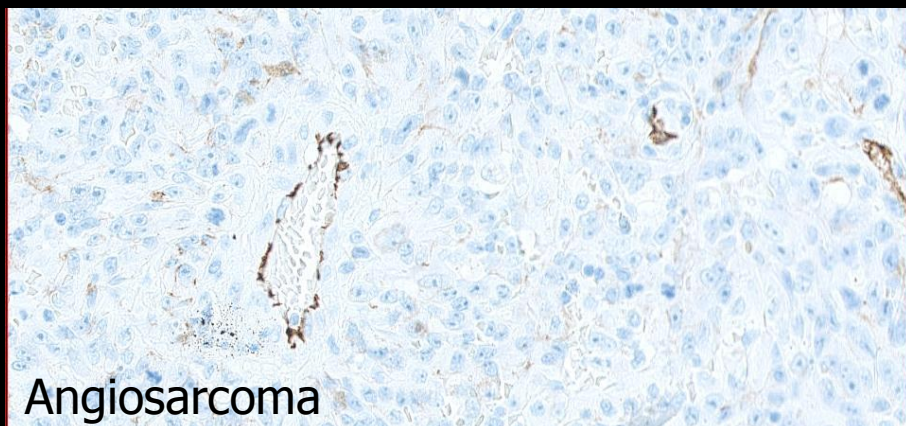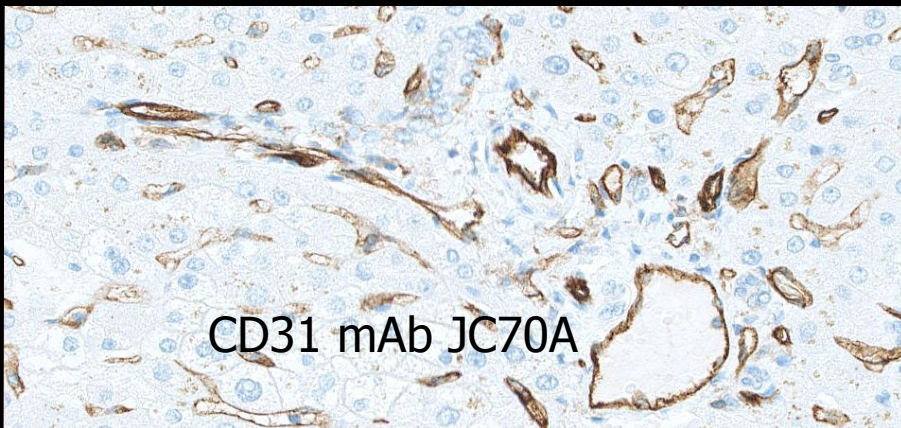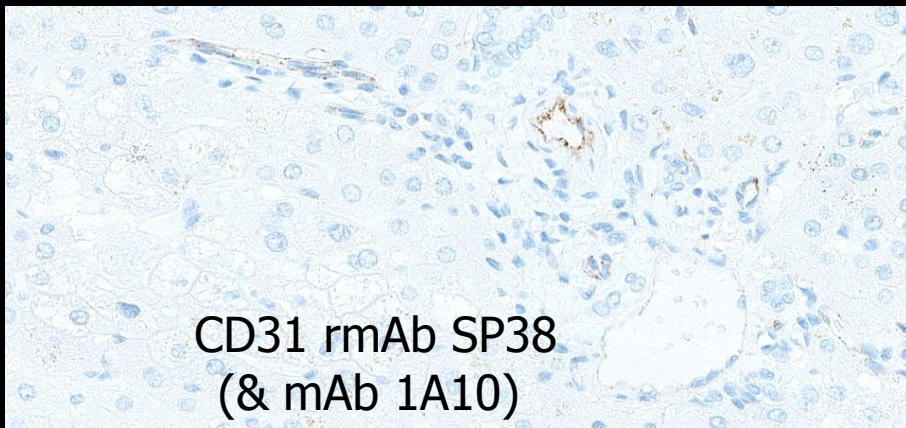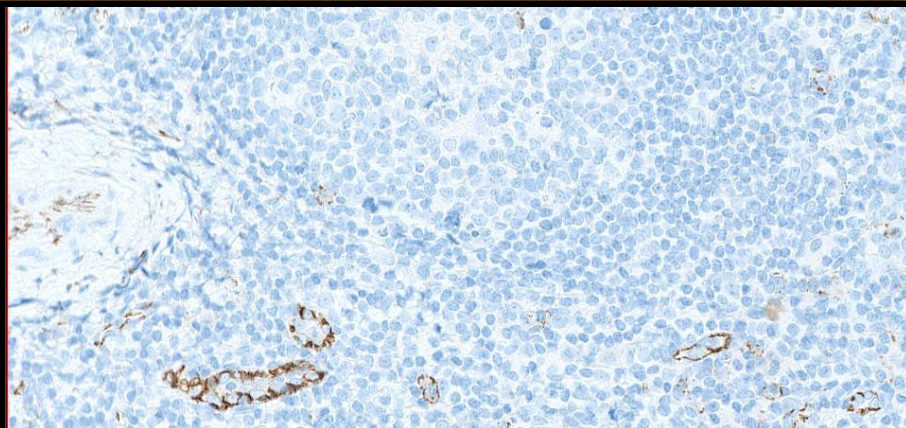

IHC – Biomarker controls

Neg. reagent control

MLH1 mAb ES05

MLH1 rmAb EPR3894

Tonsil: pos. control
Carc. with loss: neg. control


Reduced titre.....

■ Analytical validation – Challenges


- Expected level of high, intermediate, low and absence can be difficult to comply with e.g.
 - New marker not tested previously
 - Binary expression – yes/no (CD20) – no dynamic range
 - New IHC system changing the range
 - Next Generation, Dako – TSA amplification, VMS
- Number of samples
 - TMA or whole sections (homogenous / heterogenous)
 - Normal tissues or neoplasias
 - Rare positive cases (ALK lung carcinoma)

IHC – Biomarker controls



New IHC system changing the range – TSA based (OptView+A)

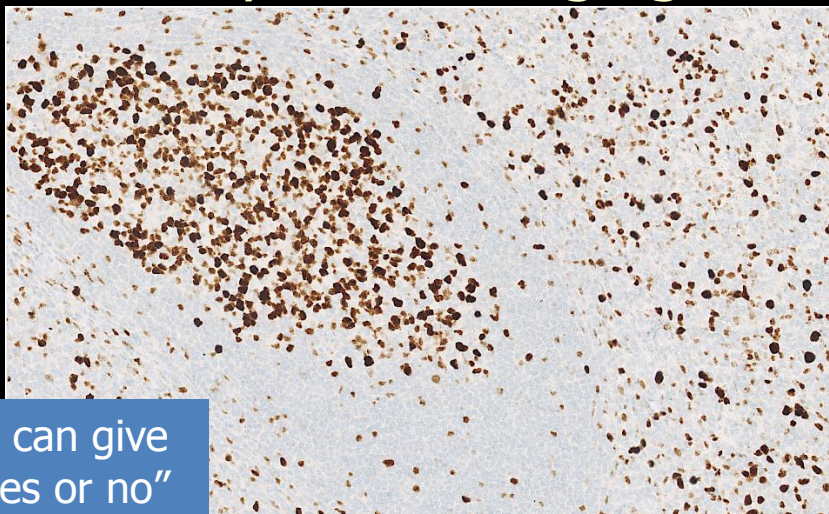

TSA can give a "yes or no" expression range

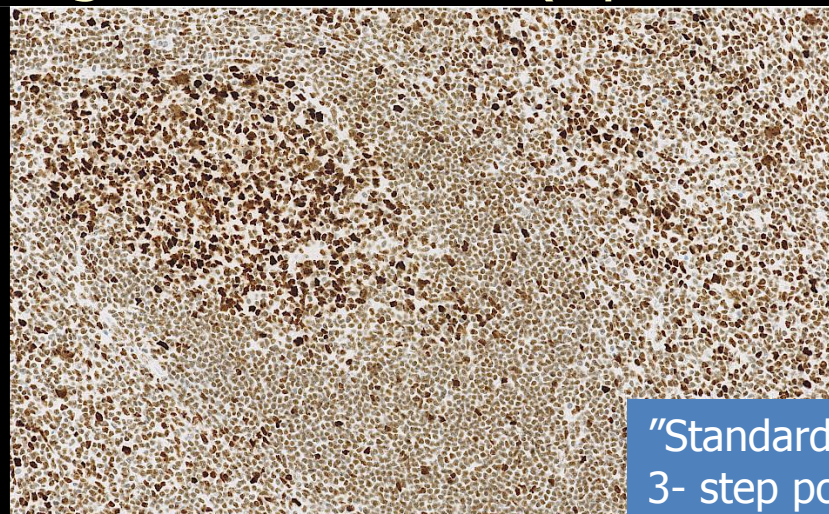



"Standard" 2- & 3- step polymer giving a dynamic range

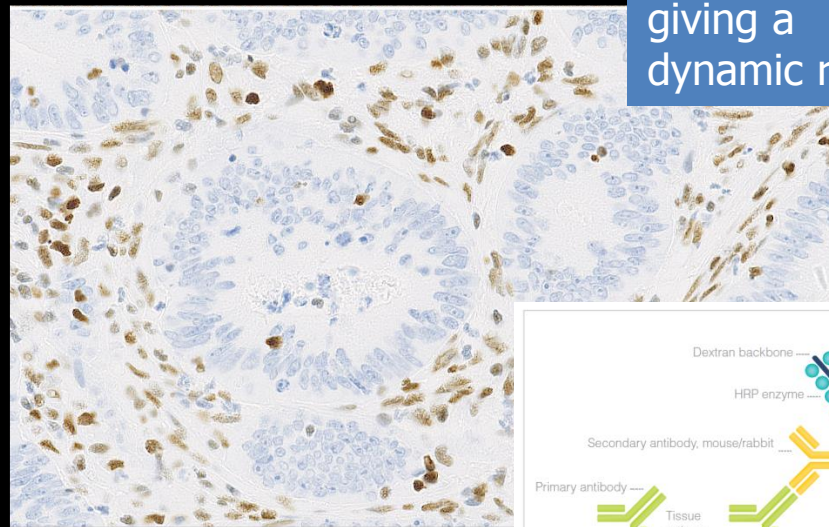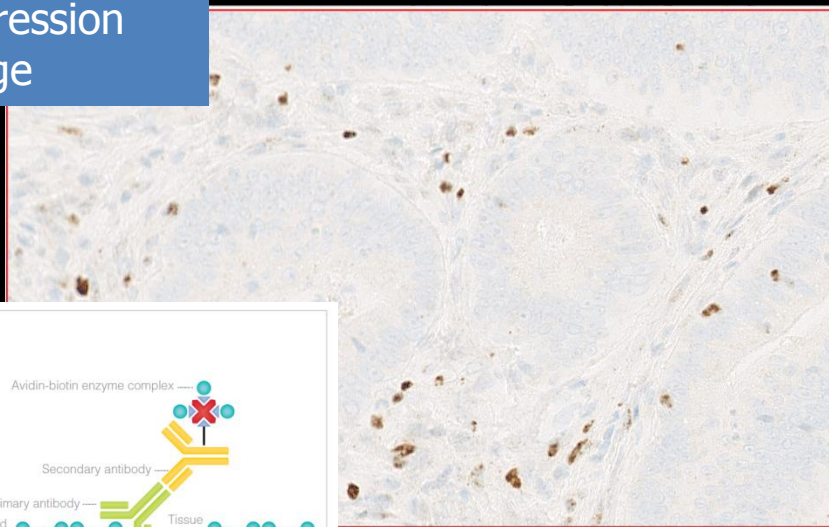

MSH6 rmAb EP49


1:200 OptiView + Amp

1:50 OptiView

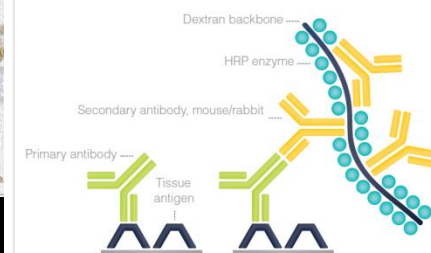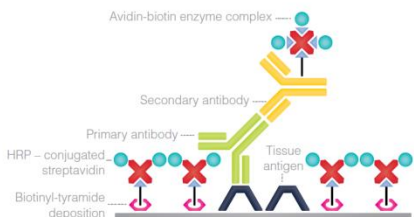

Challenge: Rare in cancers and/or in benign cells


- ALK, ROS1, PD-L1 etc and many molecular derived targets
- Needed to verify IHC method is working
 - *ALK lung; 30 cancers used to find 1 pos case.....*

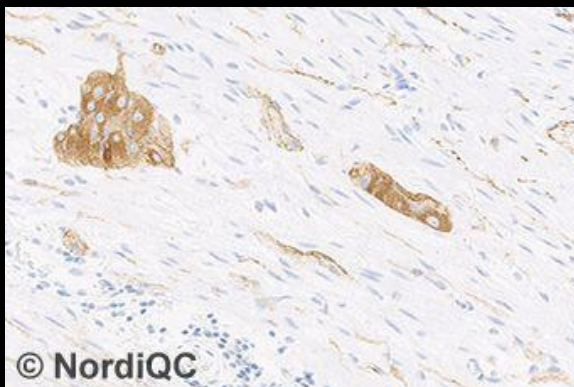

ALK

Appendix / Colon:

Peripheral nerves – axons and ganglion cells

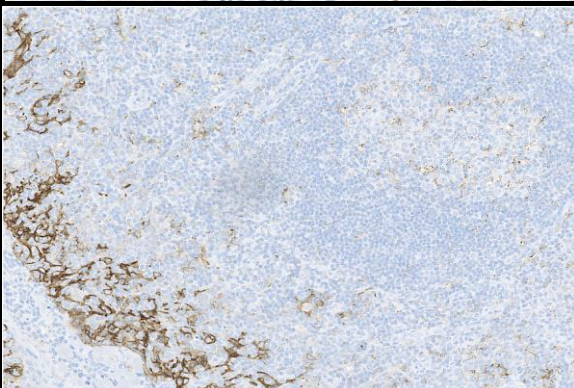

PD-L1

Tonsil:


Germinal centre macrophages



Precision and metrics of test to be confirmed

- Analytical validation – Challenges
 - New marker not tested previously
 - Search literature, pubmed etc
 - Identify tissues with and without expression
 - Normal or only neoplastic, Cell lines, etc
 - Localization – nuclear, membrane, etc
 - How to interpret – cut-off, qualitative, quantitative ?
 - Define potential clinical/diagnostic utility
 - Define other assays to be used for validation

www.antibodypedia.com

[About Us](#) | [Contact](#) | [FAQ](#) | [For Providers](#) | [Sign in](#)



[Explore](#)  [Validate](#)  [Learn](#)

[Search help](#)

Search for

Search



Advanced search ▶

e.g. [Her2](#), [Transcription factors](#), [Chromosome X](#)

Using Antibodypedia

1. **Search and identify** gene / protein target
2. **Compare and Select** antibodies
3. **Explore** antibody features and validations

Antibodypedia in focus

- [Read our newsletter and blog posts](#)
- [Visit our Facebook page](#)  

Sign up for our newsletter

Sign up

Version 8 - May 2013
Content updated 2015-04-08
1817146 reviewed antibodies from [62 providers](#),
covering gene-products encoded by [19451 genes](#)


Welcome

Welcome to Antibodypedia, an open-access database of publicly available antibodies against human protein targets. The site features user and provider data on antibody efficacy in a range of biochemical and cell biological techniques--so you can find the right antibody for the right application.

News

8 April 2015

- A warm welcome to our newest provider: Aalto Bio Reagents
- **New Antibody Market Report: Use trends and insights to improve your business in 2015!**
Antibodypedia has worked in conjunction with Pivotal Scientific Ltd to create the third Antibody Market Report giving a review of 2014 and predictions for 2015, detailing the top genes

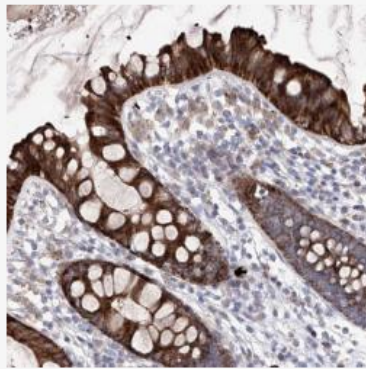



Immunohistochemistry-Paraffin: KLHDC8A Antibody [NBP1-84604] - Staining of human colon shows strong cytoplasmic positivity in glandular cells.
[More info](#)


IHC – Biomarker controls

www.antibodypedia.com

antibodypedia

 Explore

 Validate

 Learn



BRAF gene product

BRAF1

This gene encodes a protein belonging to the raf/mil family of serine/threonine protein kinases. This protein plays a role in regulating the MAP kinase/ERKs signaling pathway, which affects cell division, differentiation, and secretion. Mutations in this gene are associated with cardiofaciocutaneous syndrome, a disease characterized by heart defects, mental retardation and a distinctive facial appearance.

[More gene data](#) ▶

FEATURED ANTIBODIES

 Biorbyt	orb38546	0 references	Polyclonal	WB ● IHC ● ICC ● FC ●
 antibodies-online	ABIN968991	2 references	Monoclonal	WB ● IHC ● EL ●

ANTIBODIES

Compare Selected

863 antibodies from 32 providers.

Show Additional Columns ▶

Filters

Application

Reference

Provider

Host

Reactivity

<input type="checkbox"/>	ANTIBODY	REFS	TYPE	WB	EL	ICC	IP	IHC	FC
Santa Cruz Biotechnology 1 antibody									
<input type="checkbox"/>	sc-5284	8	Monoclonal	●				●	
Abnova Corporation 30 antibodies ▶									

www.proteinatlas.org

THE HUMAN PROTEIN ATLAS

ABOUT & HELP




A Tissue-Based Map of the Human Proteome

Here, we summarize our current knowledge regarding the human proteome mainly achieved through antibody-based methods combined with transcriptomics analysis across all major tissues and organs of the human body. A large number of lists can be accessed with direct links to gene-specific images of the corresponding proteins in the different tissues and organs.

[Read more](#)




TISSUE ATLAS



SUBCELL ATLAS



CELL LINE ATLAS



CANCER ATLAS

SEARCH ? »

e.g. insulin, PGR, CD36

Search

[Fields »](#)

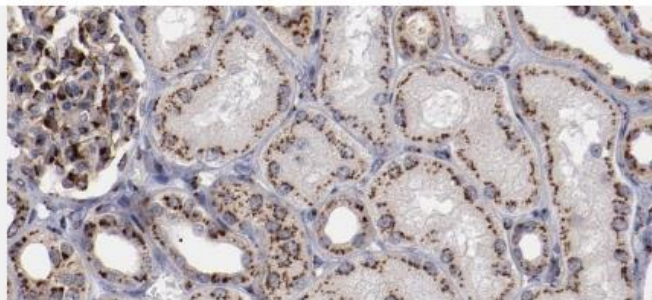


image of the day

Version: 13
Atlas updated: 2014-11-06
[release history](#)

Transcriptome analysis based on
213 tissue and cell line samples.
Proteome analysis based on
24028 antibodies targeting
16975 unique proteins.


IHC – Biomarker controls

www.proteinatlas.org

BRAF



TISSUE



SUBCELL



CELL LINE



CANCER

GENE/PROTEIN

ANTIBODY/ANTIGEN

TISSUE ATLAS

STAINING OVERVIEW

Dictionary



Dictionary

TISSUE ATLAS

Gene description V-raf murine sarcoma viral oncogene homolog B

RNA tissue category Expressed in all.

Protein summary Detected at **High or Medium** expression levels in **51 of 81** analyzed normal tissue cell types.


Protein expression General cytoplasmic expression.

Protein class Cancer-related genes, Disease related genes, Enzymes, FDA approved drug targets

Predicted localization Intracellular

Protein evidence Evidence at protein level


Protein reliability Supportive based on 2 antibodies.




Liver



Colon



Kidney



Testis




Lymph node



Cerebral cortex

RNA


Expression (FPKM)



Organ system

Protein

Localization (score)



Liver and pancreas

Liver

Gallbladder

Pancreas

Digestive tract (GI-tract)

N/A

Oral mucosa

Salivary gland

Esophagus

Stomach

Duodenum

Small intestine

Appendix

Colon

Cell lines/Histoids:


A high valueable supplement to tissue controls:

- Rare and/or not normal occuring targets
 - ALK, ROS1, BRAF etc and other molecular derived targets
- Quantitative targets
 - ER, PR, HER2, PD-L1


Cave-out – tissue processing and biological environment different compared to histological specimen and has to be encountered

IHC – Biomarker controls


HD-C170 - IHC, NordiQC, mAb clone 5A4

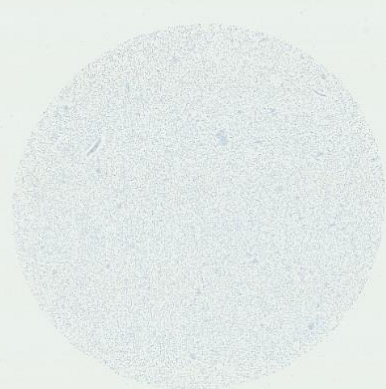

Core A

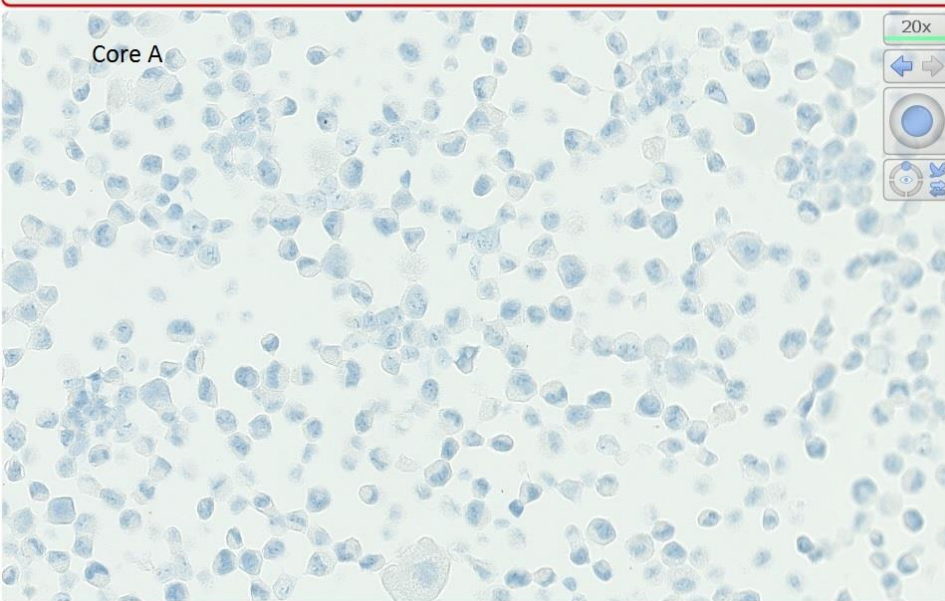

Core C

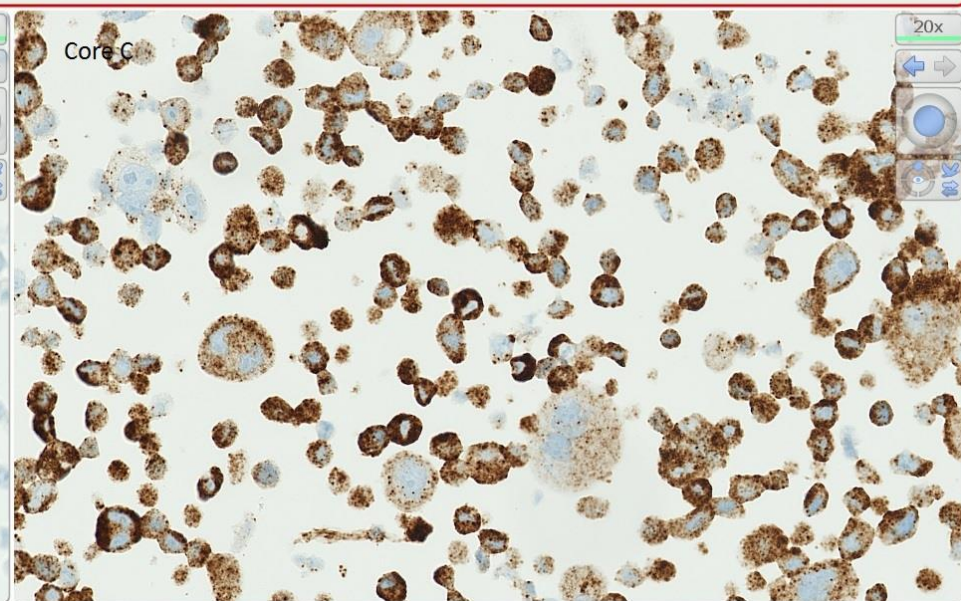

IHC – Biomarker controls

Drawing upon Horizon Discovery's proprietary genome editing platform, **GENESIS™**, Horizon Diagnostics reconstitutes clinically relevant cancer genes in human cell lines, exactly as they occur in patient tumors. Horizon Diagnostics is able to define virtually every characteristic of its reference standards, from the molecular constitution of the genome to the diameter, width and DNA output associated with each product batch. These standards have been made available in a variety of formats including **genomic DNA** aliquots, **Formalin-Fixed Paraffin-Embedded (FFPE)** slices and **fluorescent in-situ hybridization (FISH)** material. Horizon Diagnostics is also adapting the technology to support immunohistochemistry (IHC) assays.

HDx™ reference standards are already having a profound impact on the molecular labs that have adopted them:

- Validate the sensitivity and Limit of Detection (LOD) of molecular assays
- Routinely calibrate the sensitivity of assays in order to maintain quality control
- Control pre-analytical processes, including DNA extraction and quantitation using in-process standards
- Compare assay performance between platforms, assays and users from a common reference point
- Support raising standards through providing materials for staff training and proficiency schemes

www.horizondiscovery.com

horizon
precision genome editing

FREE CRISPR Reagents
for Knockout Generation

[Join the Program Now!](#)





[About us](#) | [What we do](#) | [How we can help](#) | [Working with us](#) | [Investor Relations](#) | [Talk to us](#)

[Sign in](#) | [Register](#) | [My Basket](#)

Translating genomes /
personalizing medicine



NEW PD-L1 Analyte Control with Dynamic Range of Expression



- Consistent - Reliable - Effective

Dynamic Range of expression for PD-L1 to fully demonstrate the sensitivity of your assay.

Available now from



Quality in Control

Welcome to HistoCyte Laboratories

We manufacture a range of cell line controls for same slide use in immunohistochemistry (IHC) and in situ hybridization (ISH). HistoCyte Laboratories Ltd have developed unique processes that allow the production of high density cell preparations that retain their original morphology. Through careful selection of cell types we can generate a range of positive and negative controls to determine effective performance of reagents used in slide based assessments.

Products

View our range of high quality, reliable control material



Services

We offer a range of contract services to assist in product development

- Biomarker Characterization
 - Proof of Concept
- Custom Cell Line Development
- Assay Design
- QMS Auditing

About

Learn more about our company and history



Quality in Control




Conclusions – technical calibration & analytical validation (IHC Class I)

1. IHC assay is calibrated (LD assay) / verified (RTU – plug-and-play) on TMA with 16-30 different normal tissues. If access to ICAPCs these must be included and submitted to pre-analytical conditions applied in the laboratory.
2. IHC assay is validated on TMA with e.g. 30-45 commonly seen neoplasias (analytical specificity) and 3-10 neoplasias expected to be demonstrated (analytical sensitivity).
3. Results compared to literature, reference clone etc and conclusion made.



Issues to be addressed :

1. Calibration of IHC assay and identification of best practice protocol – clone, titre, retrieval etc
2. "Evaluation of the robustness of the IHC assay – impact on pre-analytics
3. Evaluation of the analytical sensitivity/specificity
4. Identification of IHC performance controls providing information that the established level of detection is obtained in each test performed in daily practice.


Tissue controls are key element

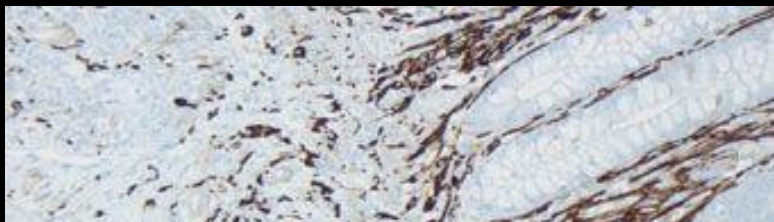

CD56: Optimal

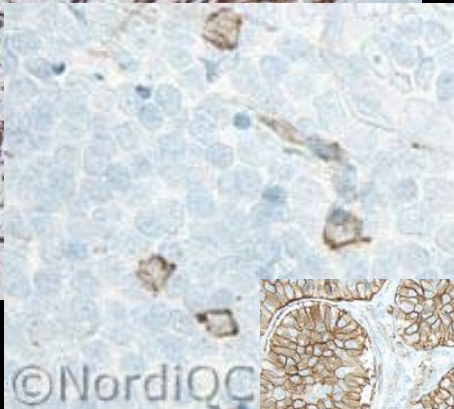

Insufficient....

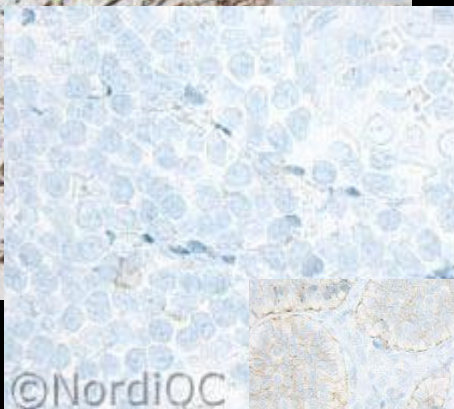

Tissues/cells with only high expression will not identify:

1. A poorly calibrated IHC assay
2. A reduced sensitivity in an optimally calibrated IHC assay

If an IHC test is used to demonstrate the target antigen being expressed at different levels, the controls must reflect this !

B1: Appendix, Hepar, Tonsil, Pancreas

CD2
CD3
CD19
CD34
CD117
CEA
CGA
CK20
DOG1
MMR
S100
SYP


ASMA
CD4
CD31
CD34
CD45
CD68
CK Pan
CK LMW
CK8
CK18
HEPA
Arginase

BCL2 MMR
BCL6 S100
CD2
CD3
CD4
CD5
CD8
CD10
CD20
CD21
CD23
CD38
CD56
CD79a
CD138
CK Pan
CyD1
EMA

CDX2
CGA
SYP
CK7
PP
SMAD4
SYP


Used together inclusive:

HE
LE
NE

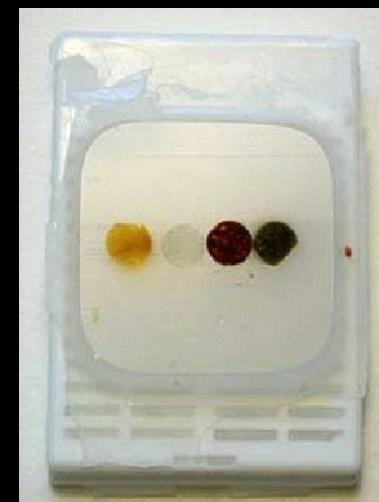


IHC – Biomarker controls

CD4 (M)	Appendix	Liver	Pancreas	Tonsil
High expression (right ab)	The majority of T-cells in lamina propria must show a moderate to strong, distinct predominantly membranous staining reaction.	The majority of T-cells, both in the interfollicular T-zones and in the germinal centres must show a moderate to strong, distinct, predominantly membranous staining reaction.	Dispersed T-cells must show a moderate to strong, distinct predominantly membranous staining reaction.	Dispersed T-cells and Kupffer cells must show a moderate to strong, distinct predominantly membranous staining reaction.-
Low expression iCAPCs (right sens.)	Dispersed intra-epithelial T-cells must show an at least weak to moderate, distinct predominantly membranous staining reaction.	The germinal centre macrophages must show an at least weak to moderate predominantly membranous staining reaction.	-	The vast majority of the endothelial cells of the liver sinusoids must show an at least weak to moderate, distinct predominantly membranous staining reaction.
Non expression (right spec.)	No staining reaction must be seen in the columnar epithelial cells.	No staining reaction must be seen in the mantle zone and germinal centre B-cells.	No staining reaction must be seen in the epithelial cells of the exocrine pancreas or the endocrine cells of the islets of Langerhans.	No staining reaction must be seen in the hepatocytes.

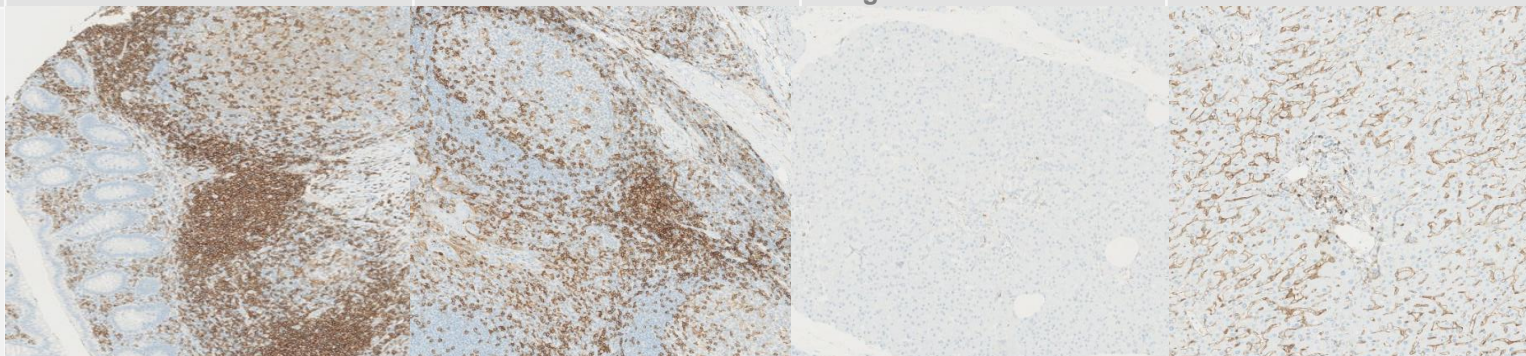

“Ideal” daily control for the majority of routine markers:

Appendix
Liver
Pancreas
Tonsil

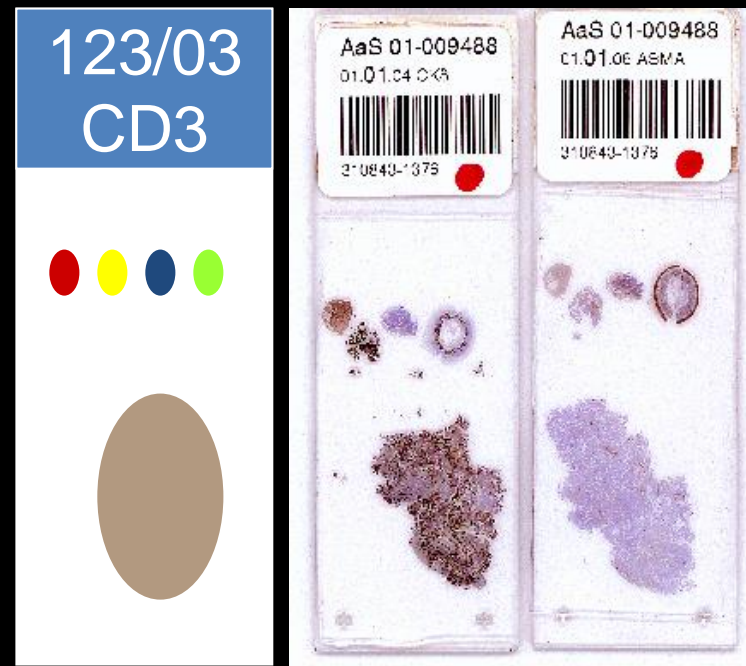

Each slide stained and evaluated has essential information of the obtained sensitivity and specificity

In contrast only using 1 external tissue run control, no information is available for the single slide evaluated₃



	TMA control on all slides	One batch control	Remarks
Missing reagent FN in patient test	Yes	No – only control slide	Potential internal pos. control only indicator of protocol performed
Wrong antibody FP in patient test	Yes	No – only control slide	
Inappropriate protocol performance - Drying out etc FN / FP in patient test	Yes	No – only control slide	Potential internal pos. control only indicator of protocol performed
	Errors seen for all IHC automated and semi-automated IHC platforms		



"Patient" 3 IHC assay level could be related to:

1. Biology
2. Tissue processing
3. Missing reagent or other technical issue

Melan-A in sex cord tumours

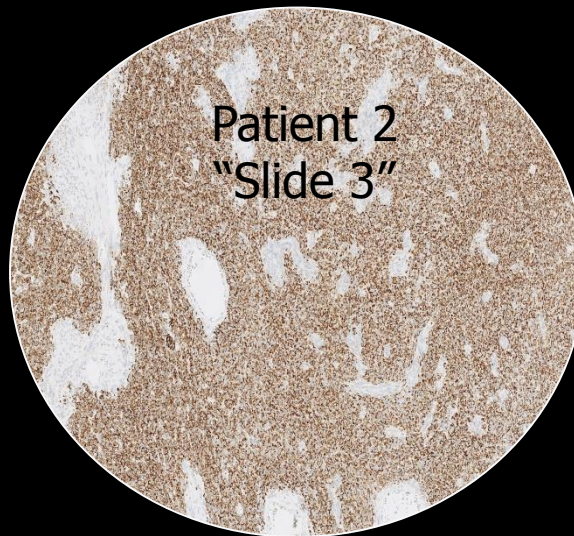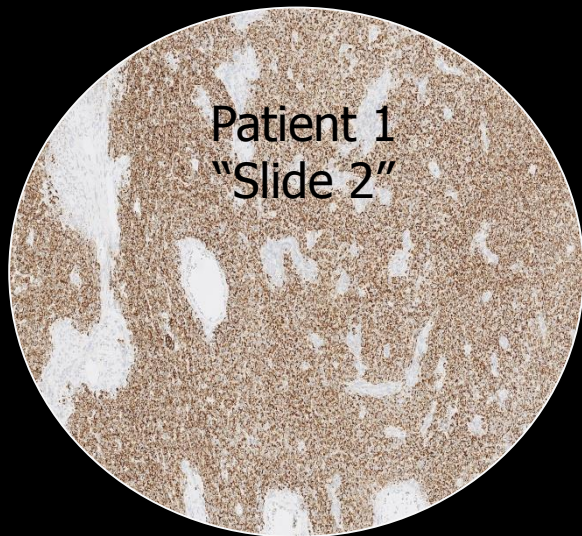

On-slide control

"Patient" 3 IHC assay level could be related to:

1. Biology
2. Tissue processing
3. Missing reagent or other technical issue

Patient 1
"Slide 1"


Patient 2
"Slide 2"

Patient 3
"Slide 3"


IHC – Biomarker controls

Consider each slide position / chamber on the IHC stainer as an individual stainer and use appropriate on-slide controls




















PCK – slide no. 1



PCK – slide no. 2



Same reagents, same protocol, same block, same stainer



Requirements to tissue control library / catalogue:

- Recommendations for virtually all markers used
 - Qualitative markers "Class I"– yes / no
 - Quantitative markers "Class II" – how much
 - "Research" markers / not established markers

Central issues to adress for control material of HER2 IHC test

1. Control material for initial calibration and validation
e.g 100 samples ranging 0, 1+, 2+, 3+.

Optimally all samples confirmed by ISH

Metrix can be generated and test implemented.

2. Control material to monitor consistent and right level of sensitivity as identified by calibration – transfer of method – is obtained in each test performed.

Focus: The issue to identify and use proper control material to monitor consistency of test

Central issues to adress for control material of HER2 IHC test


In NordiQC app. 60-70% of laboratories use a 3+ tumour as routine positive control for HER2 IHC



Question:


Is this reliable to monitor a consistent level of HER2 assay ?

IHC – Biomarker controls

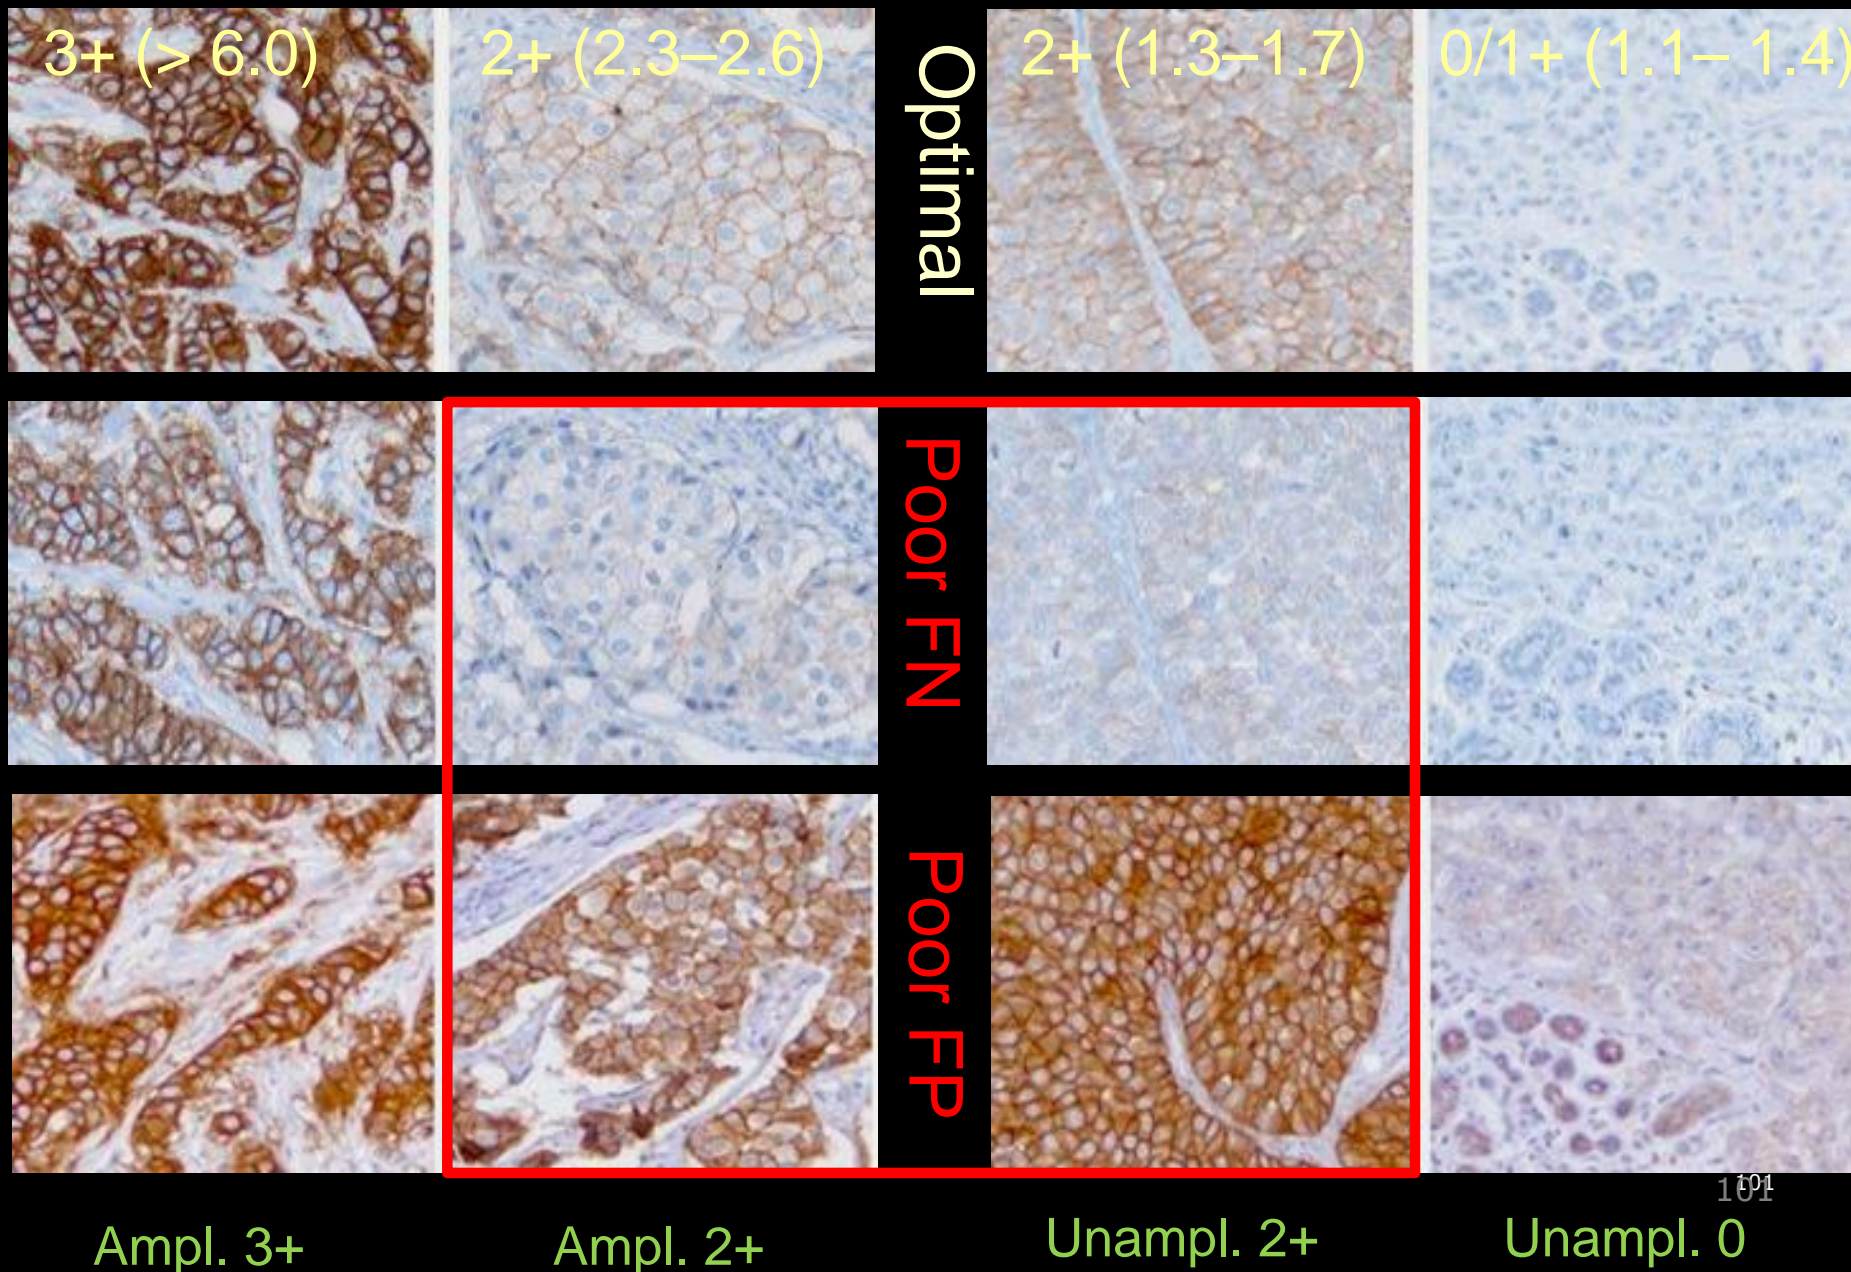


PATHWAY 1

CC1_64/32M/OP


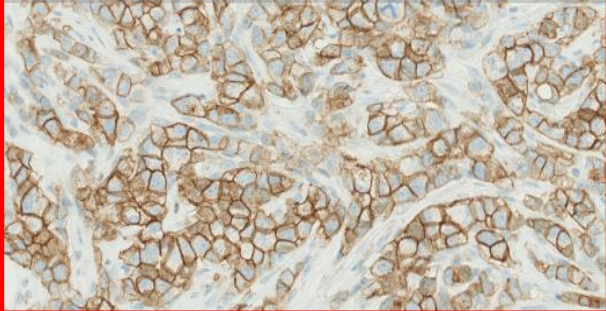


PATHWAY 2

CC1_32/16M/UV

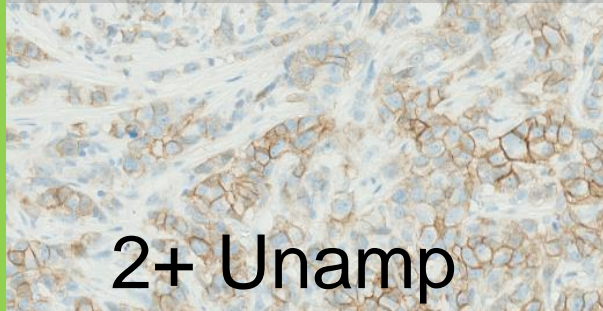





2+ Unamp

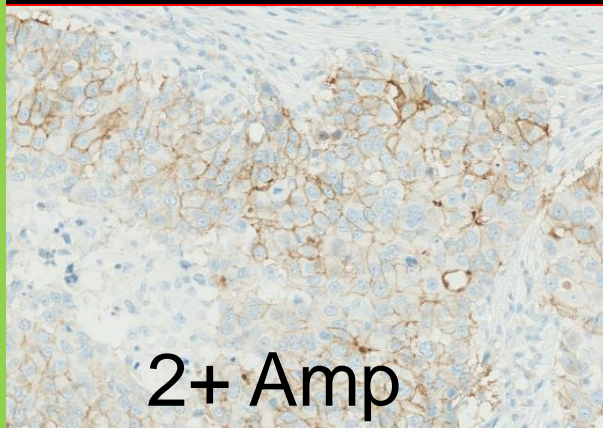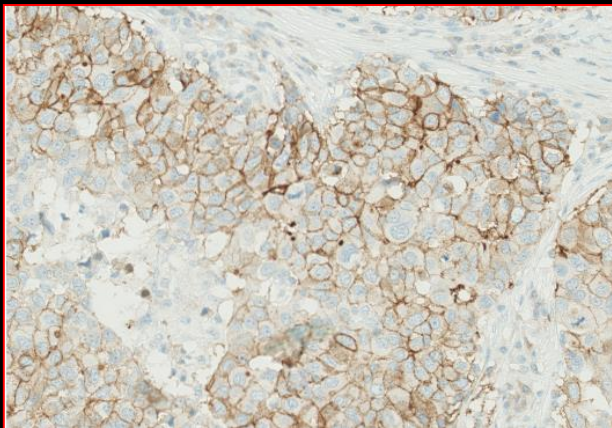


2+ Amp

PATHWAY 3

CC1_24/12M/UV

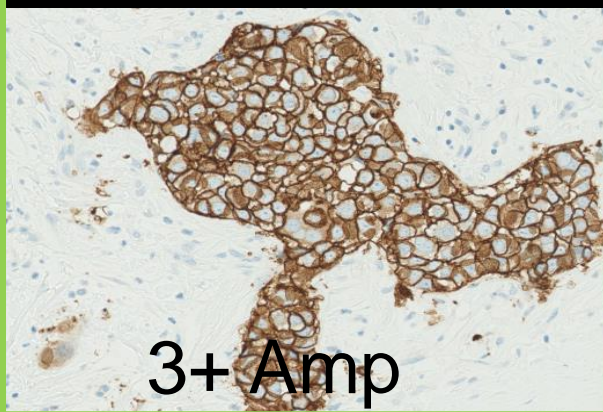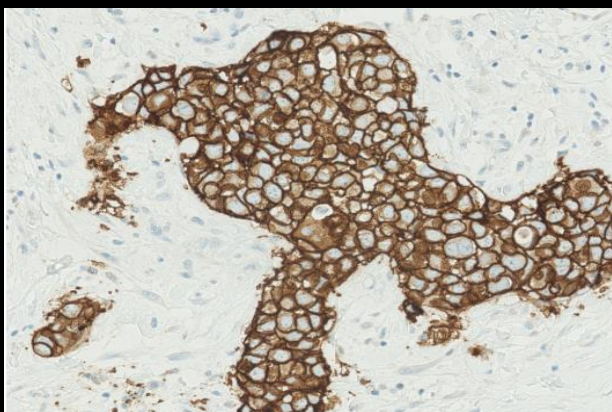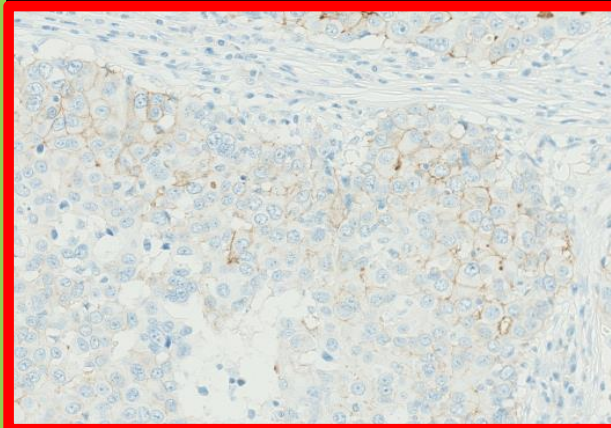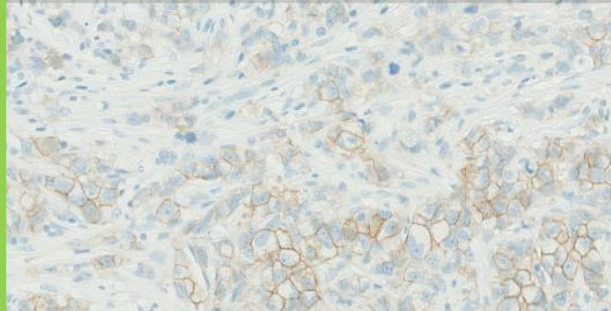


3+ Amp

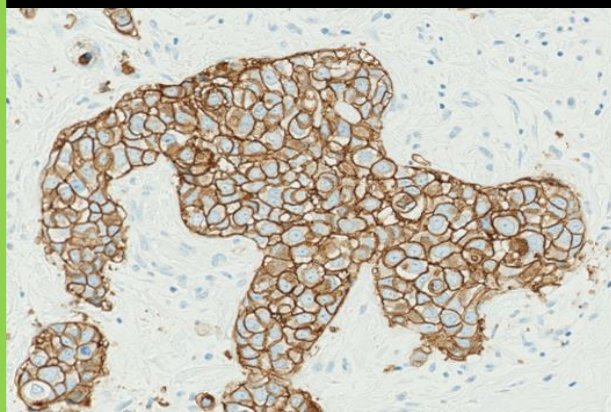

Central issues to address for control material of HER2 IHC test

In NordiQC app. 60-70% of laboratories use a 3+ tumour as positive control for HER2 IHC

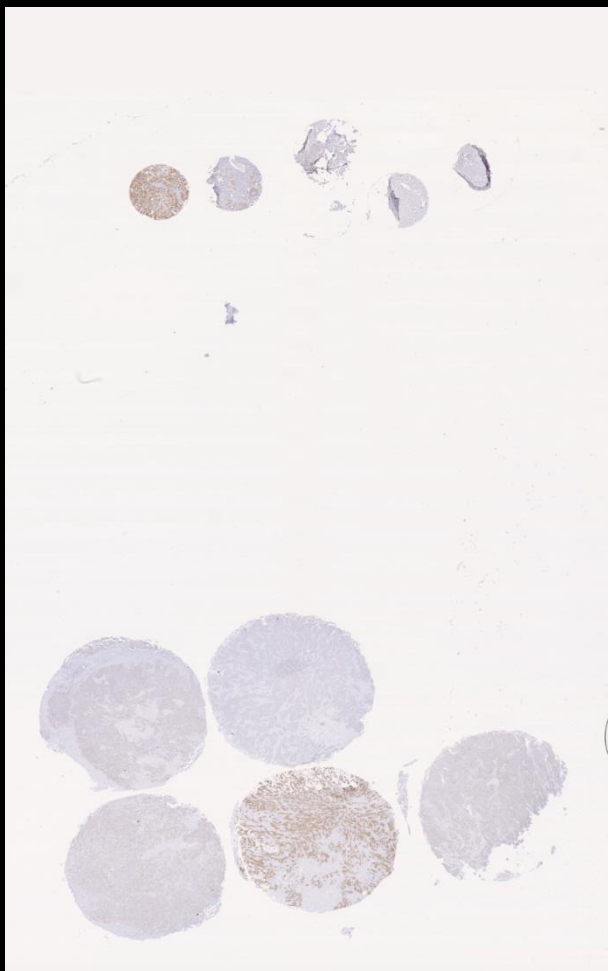


Optimally:

Use small TMA
with 1+, 2+ & 3+
mounted on
same slide as pt
material for daily
control of HER2
IHC assay

IHC scoring system according to the 2013 ASCO/CAP guidelines




Score 0	No staining is observed or incomplete membrane staining is observed in $\leq 10\%$ of the tumour cells.
Score 1+	A faint perceptible and incomplete membrane staining is observed in more than 10% of the tumour cells.
Score 2+	A weak to moderate circumferential incomplete membrane staining is observed in more than 10% of the tumour cells or an intense circumferential complete membranous staining in $\leq 10\%$ of the tumour cells.
Score 3+	An intense circumferential complete membrane staining is observed in more than 10% of the tumour cells.

- What is faint ?
- What is weak ?

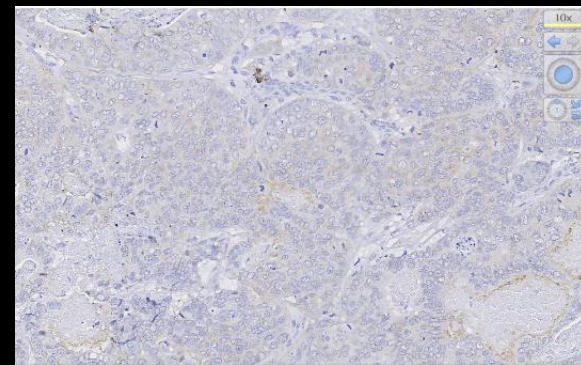

Up to 20-40% HER2 IHC tests are reflexed to ISH
due to expanded criteria for 2+ (internal data)

IHC – Biomarker controls

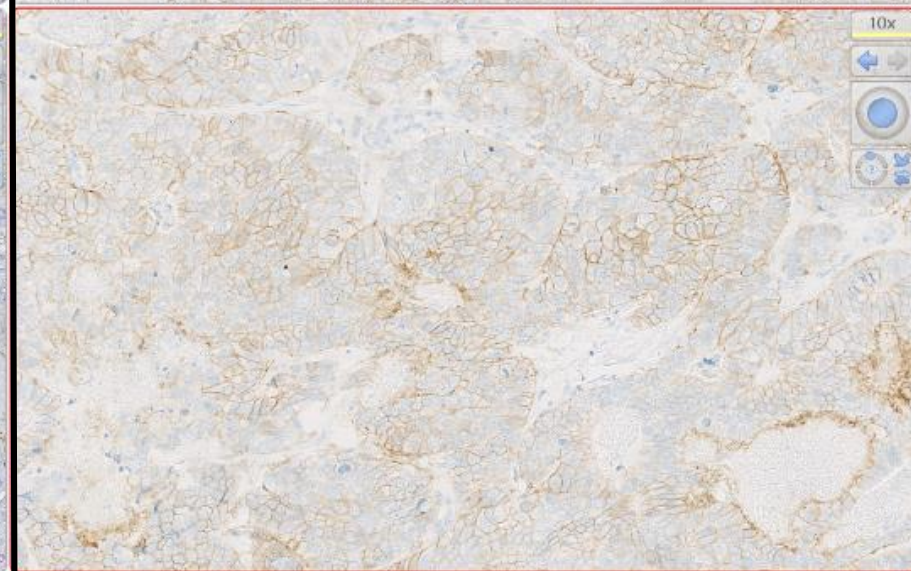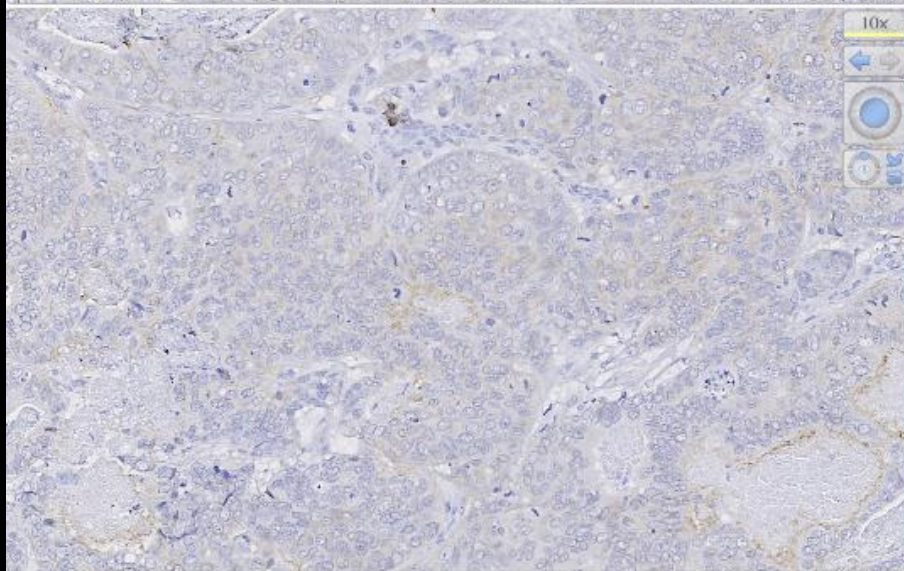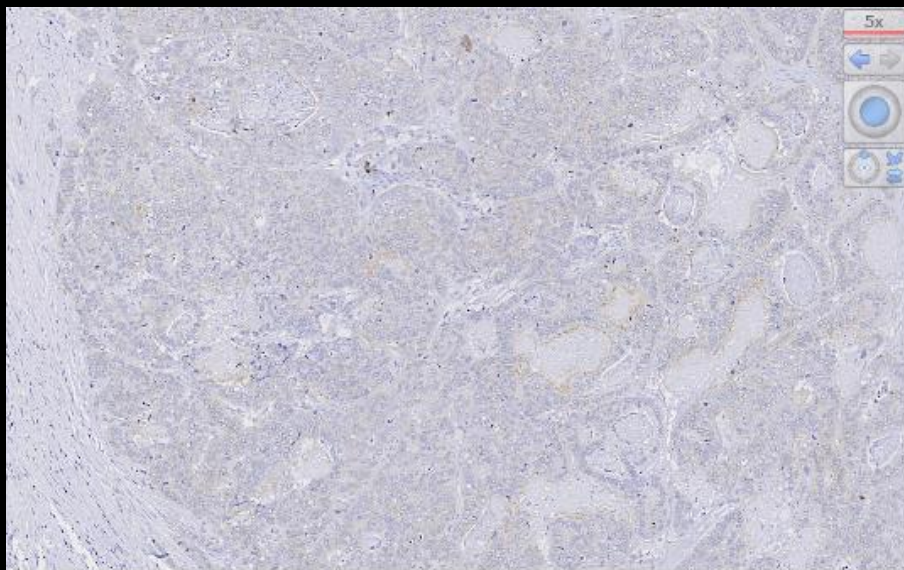

Lab 1; scored 2+

Lab 2; scored as 2+

Histopathology




Histopathology 2012, 60, 758–767. DOI: 10.1111/j.1365-2559.2011.04142.x


ImmunoMembrane: a publicly available web application for digital image analysis of HER2 immunohistochemistry

Vilppu J Tuominen,¹ Teemu T Tolonen^{1,2} & Jorma Isola¹

¹*Institute of Biomedical Technology, University of Tampere, Tampere, Finland, and* ²*Department of Pathology, Centre for Laboratory Medicine, Tampere University Hospital, Tampere, Finland*

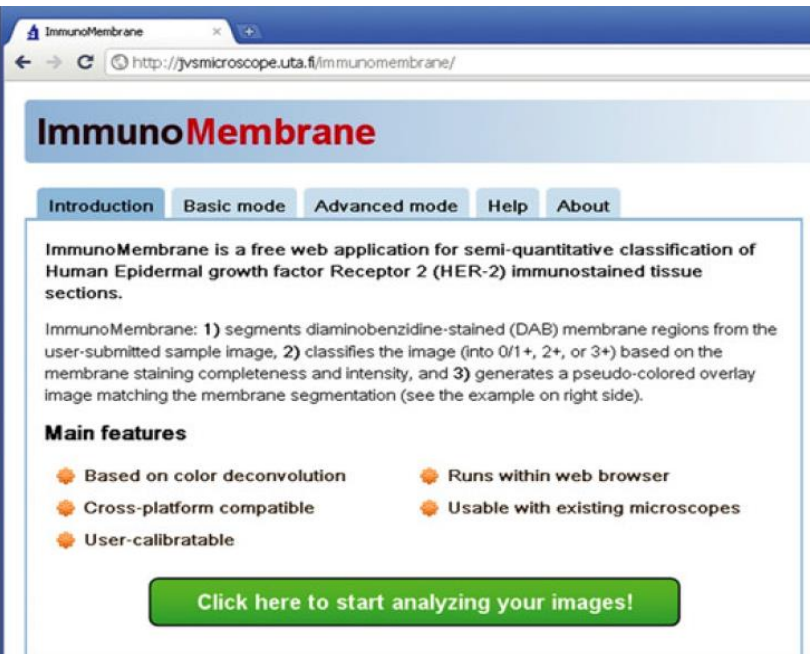

The screenshot shows the ImmunoMembrane web application interface. At the top, there is a browser address bar showing the URL <http://jvsmicroscope.uta.fi/immunomembrane/>. Below the address bar, the title "ImmunoMembrane" is displayed in a blue header. Underneath the title, there are navigation tabs: "Introduction", "Basic mode", "Advanced mode", "Help", and "About". The "Introduction" tab is selected. The main content area contains a paragraph describing the application: "ImmunoMembrane is a free web application for semi-quantitative classification of Human Epidermal growth factor Receptor 2 (HER-2) immunostained tissue sections." Below this, there is a detailed description of the application's workflow: "ImmunoMembrane: 1) segments diaminobenzidine-stained (DAB) membrane regions from the user-submitted sample image, 2) classifies the image (into 0/1+, 2+, or 3+) based on the membrane staining completeness and intensity, and 3) generates a pseudo-colored overlay image matching the membrane segmentation (see the example on right side)." A section titled "Main features" lists four bullet points: "Based on color deconvolution", "Cross-platform compatible", "User-calibratable", and "Runs within web browser". Below the list, there is a green button that says "Click here to start analyzing your images!".

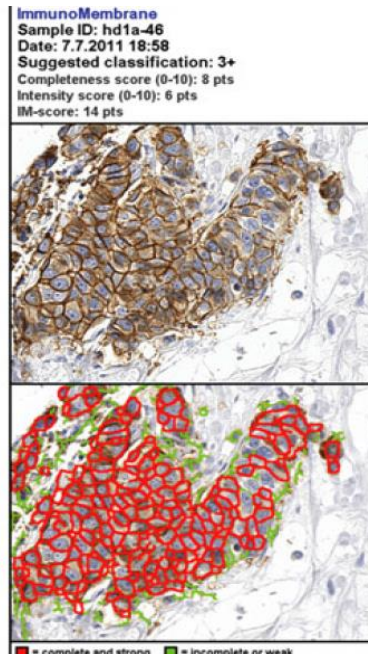

Digital computer assisted analysis to be integrated.


IHC – Biomarker controls

Automated image analysis is superior to manual reading of HER2 expression in breast cancer

Rossing HH, Talman ML, Vainer B

Department of Pathology, Rigshospitalet, University of Copenhagen, Denmark


Aim: Validate digital, automated image analysis algorithm HER2-CONNECT, with a goal to minimizing the number of inconclusive HER 2+ scores.

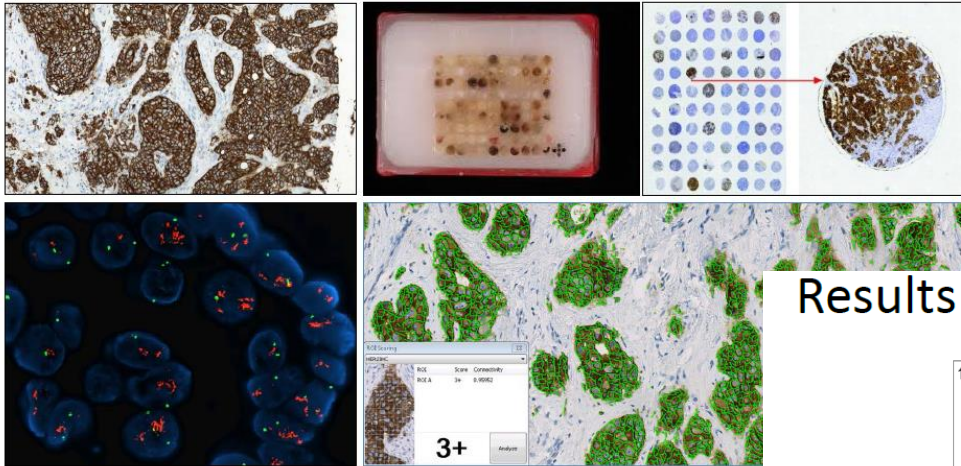

156 patients in 12 TMA

To improve consistency
To reduce cohort of 2+
To serve as internal QC

Results

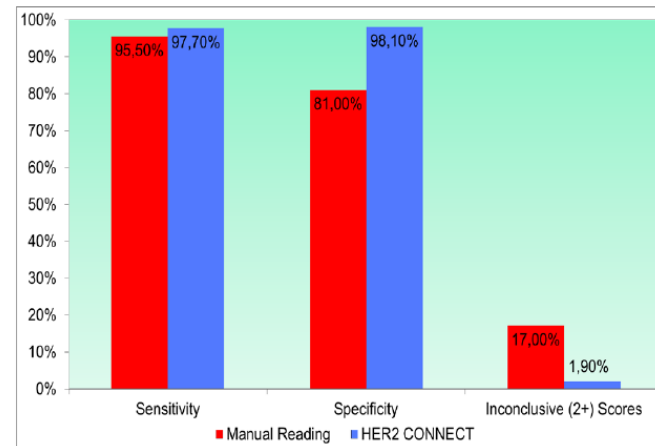

Automated image analysis HER2-CONNECT algorithm for HER2 protein expression decreased the need for supplementary FISH testing by almost 90%

HER2-CONNECT will make the assessment of HER2 fully automatic, fast and objective to the benefit of breast cancer patients.

Breast Cancer Res Treat (2012) 132:41–49
DOI 10.1007/s10549-011-1514-2

PRECLINICAL STUDY

Digital image analysis of membrane connectivity is a robust measure of HER2 immunostains

Anja Brüggmann · Mikkel Eld · Giedrius Lelkaitis · Søren Nielsen · Michael Grunkin · Johan D. Hansen · Niels T. Foged · Mogens Vyberg


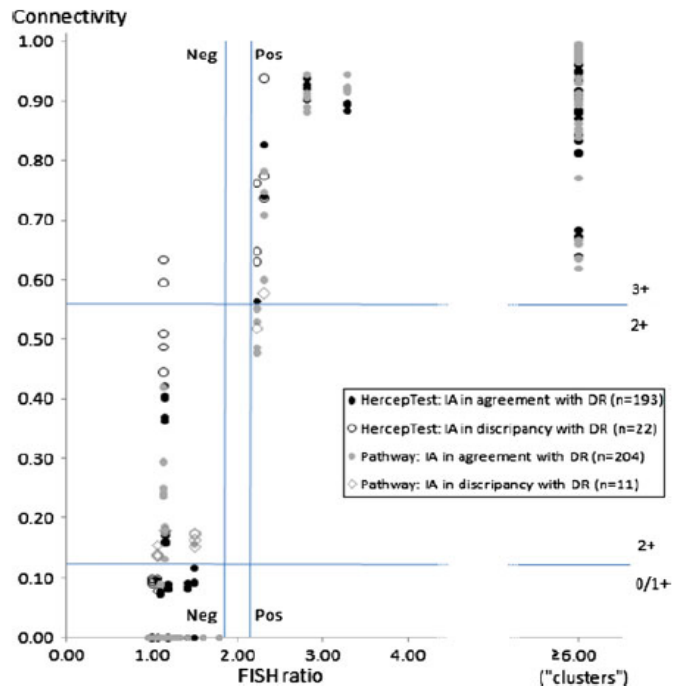


Fig. 4 HER2 connectivity versus FISH ratio. The blue lines on the x axis define the “equivocal” category with FISH ratio between 1.8 and 2.2. The FISH ratios lower than 1.8 are negative (Neg) and above 2.2 are positive (Pos). On the y axis the blue lines define the connectivity cut-off levels separating the IHC score categories

Fig. 2 Stepwise processing of digital images by the HER2-CONNECT™ algorithm. Digital images of two fields of view from a positive (3+) (a) and an equivocal (2+) (b) sample. The major steps were pre-processing quantifying for each pixel its contribution to brown linear structure (white: high contribution, black: low contribution); the segmentation classifying the pixels which constitute brown linear structures (green overlay label), and the post-processing skeletonizing and merging the green overlay label, when a few pixels are missing in a linear structure, and removing small objects of green overlay label

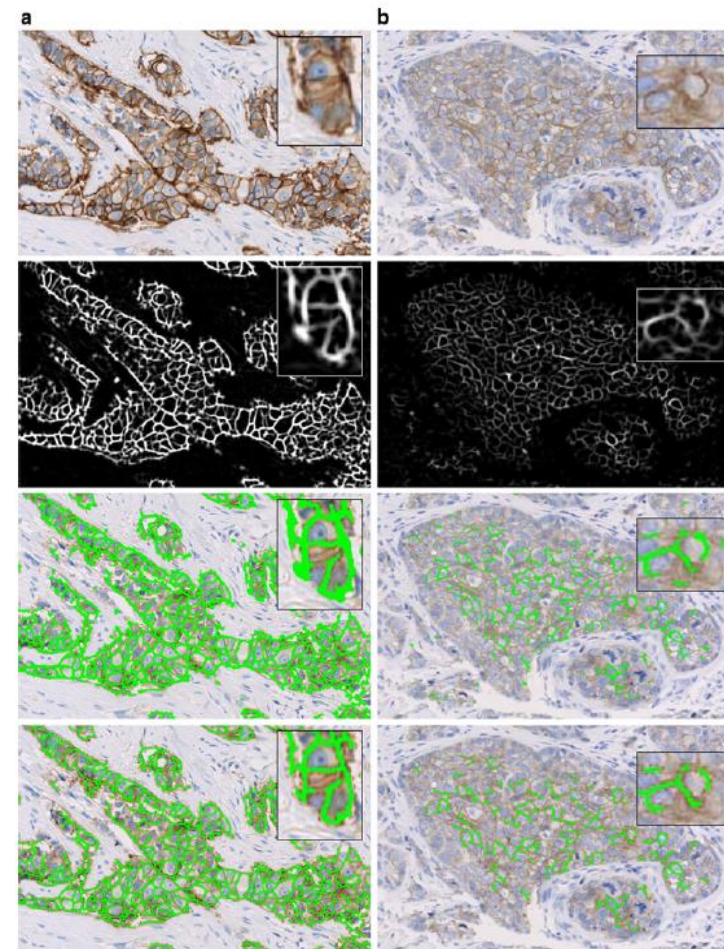

ASCO/CAP score	Connectivity Range
0	0.00
1+]0.00 - 0.40]
2+]0.40 - 0.64]
3+]0.64 - 1.00]

visiopharm
TURNING IMAGES INTO KNOWLEDGE

HER2-CONNECT™




EU: For in vitro diagnostics use

- PATHWAY
- HercepTest
- Oracle

AAS 1234_15

01.01.05

HER2

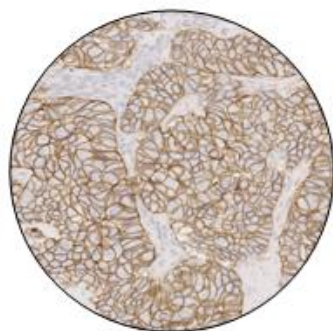

Cell line HER2

Pt HER2

	FN	Optimal	FP
CL1	< 0.20	0.20-0.30	> 0.30
CL2	< 0.40	0.40-0.50	> 0.50

ASCO/CAP score	Connectivity Range
0	0.00
1+]0.00 - 0.40]
2+]0.40 - 0.64]
3+]0.64 - 1.00]

PATHWAY 1

PATHWAY 2

PATHWAY 3

CC1_64/32M/OP

CC1_32/16M/UV

CC1_24/12M/UV

CL 1

1+ Unamp

CONNECT: 0.40

CONNECT: 0.25

Range 0.20-0.30

CONNECT: 0.10

CL 2


2+ Amp

CL 3

3+ Amp



PATHWAY 1

CC1_64/32M/OP

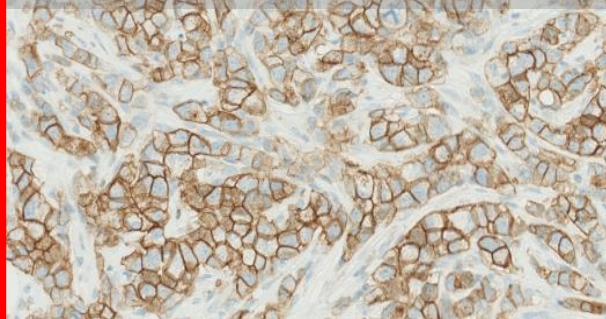


CONNECT: 0.40

CL 2

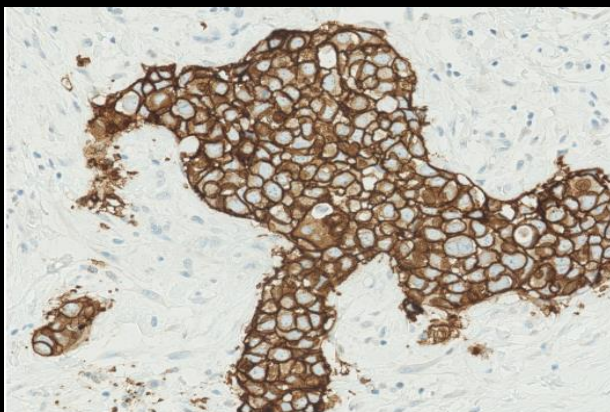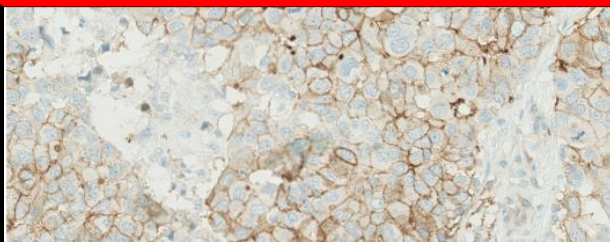

PATHWAY 2


CC1_32/16M/UV

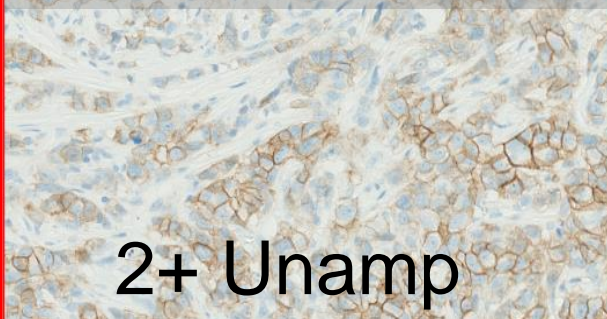


2+ Unamp

CONNECT: 0.25

Range 0.20-0.30

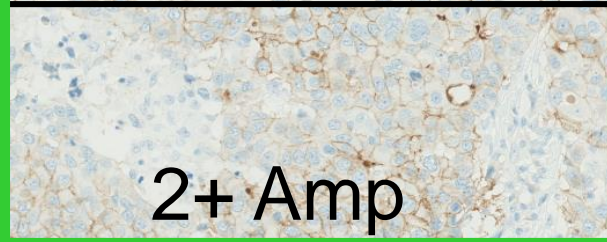


2+ Amp

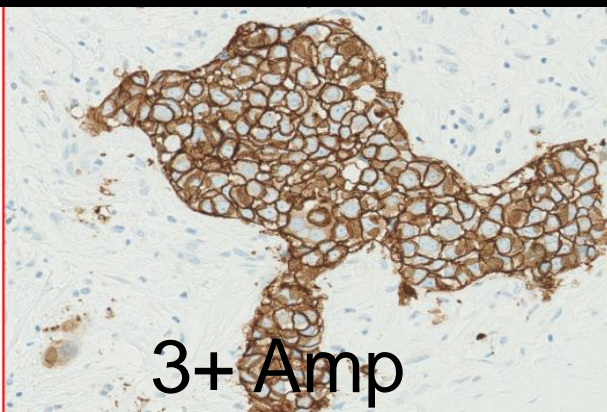



3+ Amp

PATHWAY 3

CC1_24/12M/UV

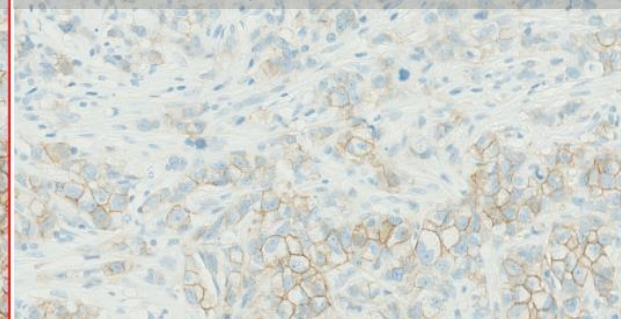

CONNECT: 0.10

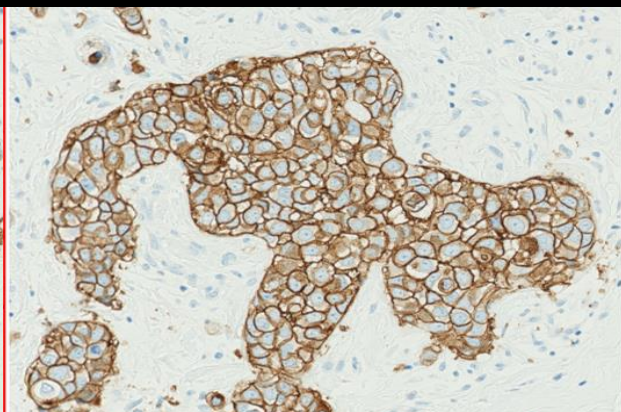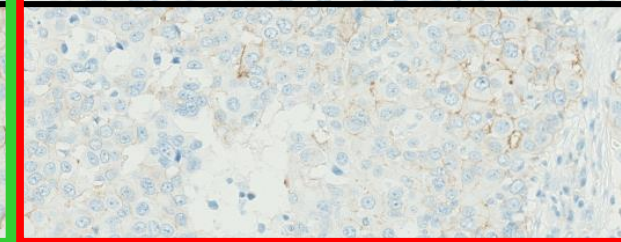

Requirements to tissue control library / catalogue:

- Recommendations for virtually all markers used
- Quantitative markers – how much
 - External tissue controls to confirm right ab
 - External tissue controls to guide level of detection
 - External cell lines with documented reference values as final QC

IHC – Biomarker controls

Standardisation of external tissue controls enables a more objective evaluation of IHC assay consistency and potential trouble shooting.

The area still needs to be improved and requires surveillance and registration of IHC results of the controls

E.g. registration of aberrant staining results in controls

Ab	Slide	Weak	FN	PS	FP	Accept	Retest
CK5	144001	+				+	
CD10	144780		+				+
MLH1	144899			+			

Or scoring of all controls

Ab	Slide	0 negative	1 weaker	2 standard	3 stronger
CK5	144001			+	
CK5	144210		+		

Conclusions:

Controls are essential to evaluate IHC results:

- Tissue controls used to calibrate IHC assay
- Tissue controls processed by variables applied in the laboratory is needed to evaluate on robustness
- Tissue controls to evaluate analytical potential
- Tissue controls to monitor consistency of IHC assay

Conclusions:

Focus on external tissue controls are central to standardize and optimize IHC:

- External tissue control "catalogue" (normal preferable) with descriptions of HE, LE and NE
- Accepted and developed by KOL, EQA, Industry, Labs
- Used to validate/verify IHC studies and publications
- Used for both internal and external IHC QC

Conclusions:

Focus on external tissue controls is central to standardize and optimize IHC:


- On-slide TMA controls are preferable to 1 batch control
- Internal tissue controls are of limited value
- Negative reagent controls are only essential for biotin-based detection systems
- Negative reagent controls can be valueable for non-biotin based systems e.g. If pigment, frozen sections..

Conclusions:

Focus on cell lines to improve level of information:

- Cell lines to be used as supplement to tissue controls for precise information of the limit of detection or threshold of sensitivity for the test performed
- Reference data for optimal performance and level of sensitivity.
- Used in combination with image analysis.

"SORRY. WERE YOU SLEEPING?"

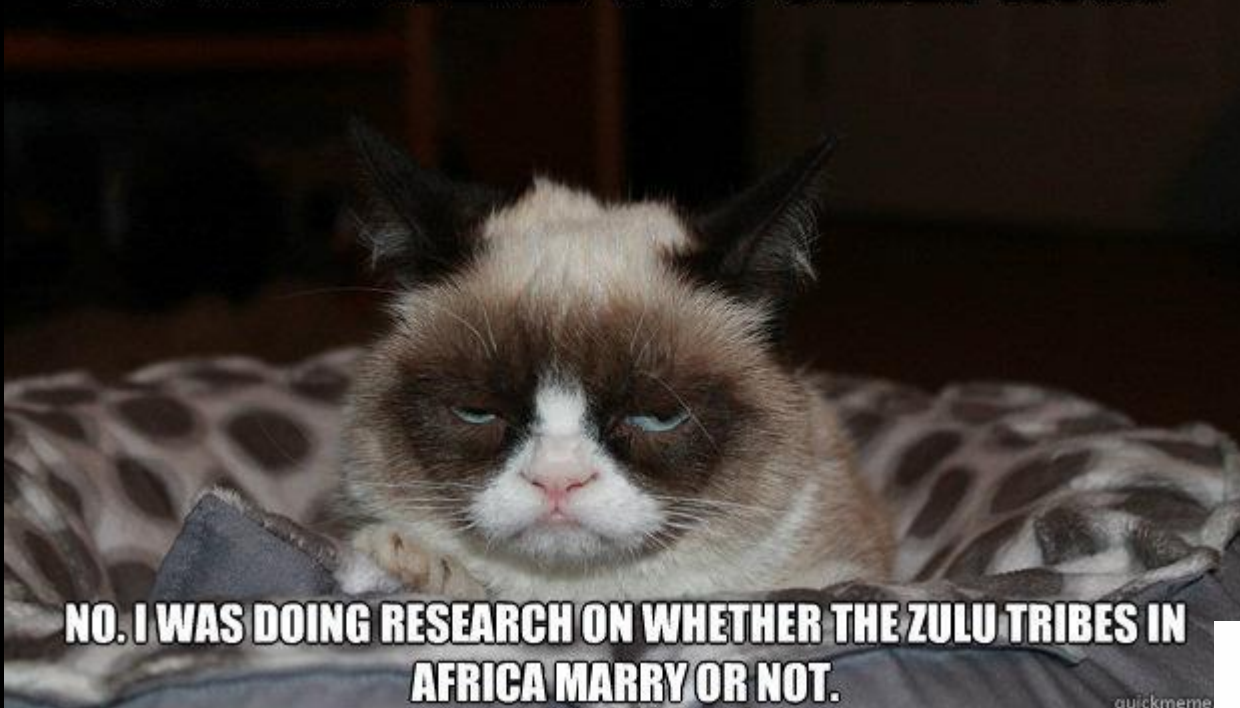

Thank You for the
attention and.....

